
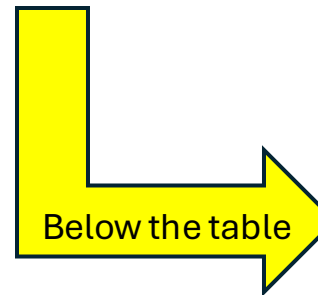
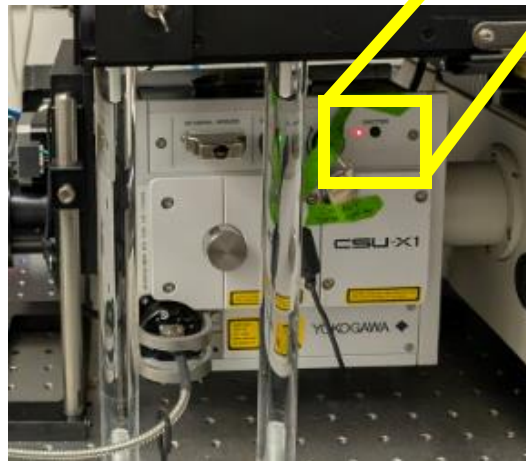
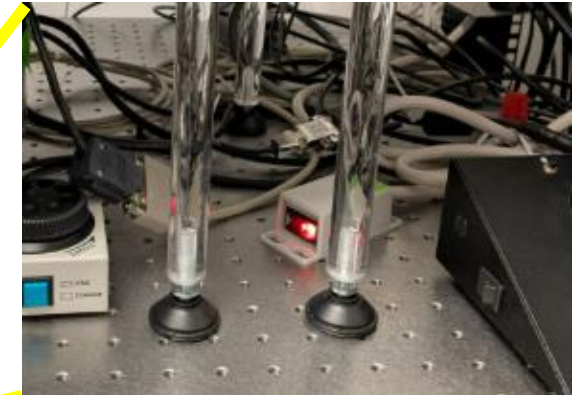
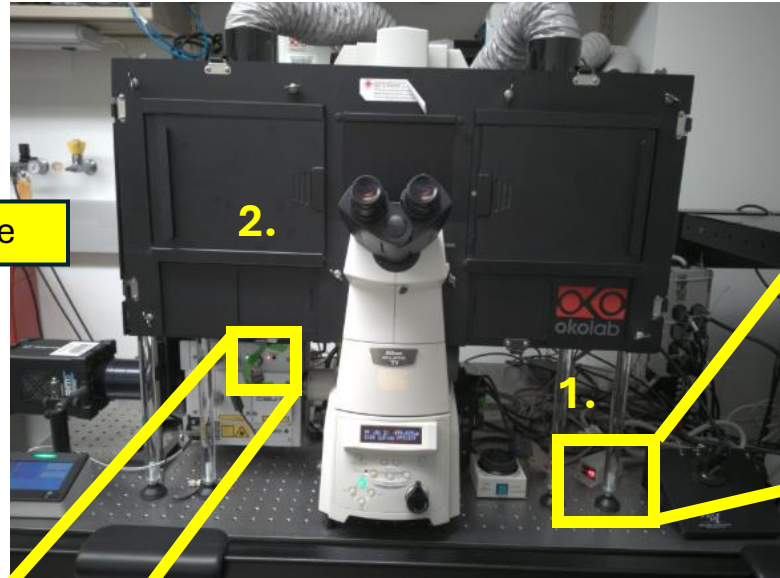


Turn ON Procedure for SD#1

1. Master Power →
2. CSU-X1 Shutter Button →
3. Turn Laser Key →
4. Make Sure Sola Power light is on →
5. Wait for camera light to stop blinking before turning on software (*don't touch camera power switch*)

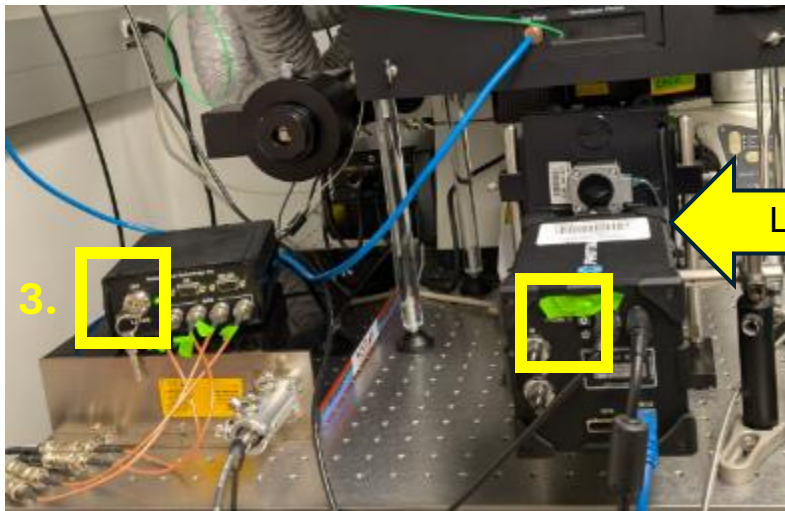

Turn OFF Procedure for SD#1

1. Close software →
2. Clean up the microscope →
3. Turn Laser Key →
4. Master Power →
5. Take your data with you