Light Sources for Microscopy

Focus on Fluorescence Microscopy

Regan Baird, Ph.D.

Jablonski Diagram

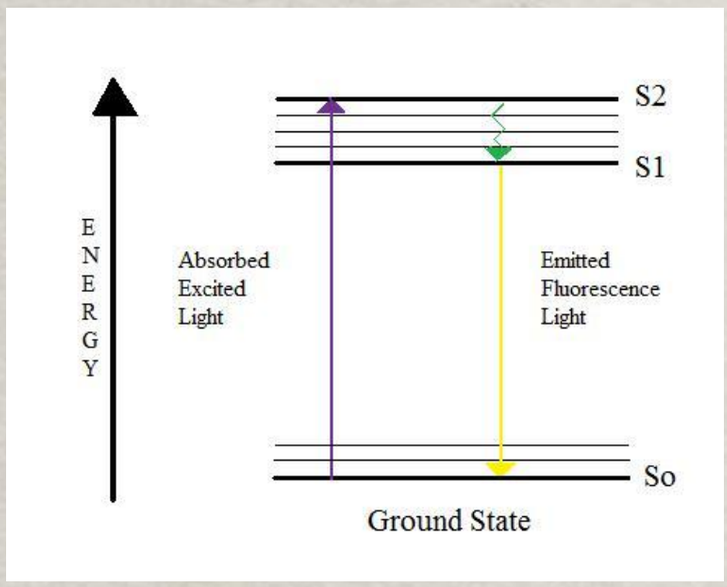

Fluorescence Spectra

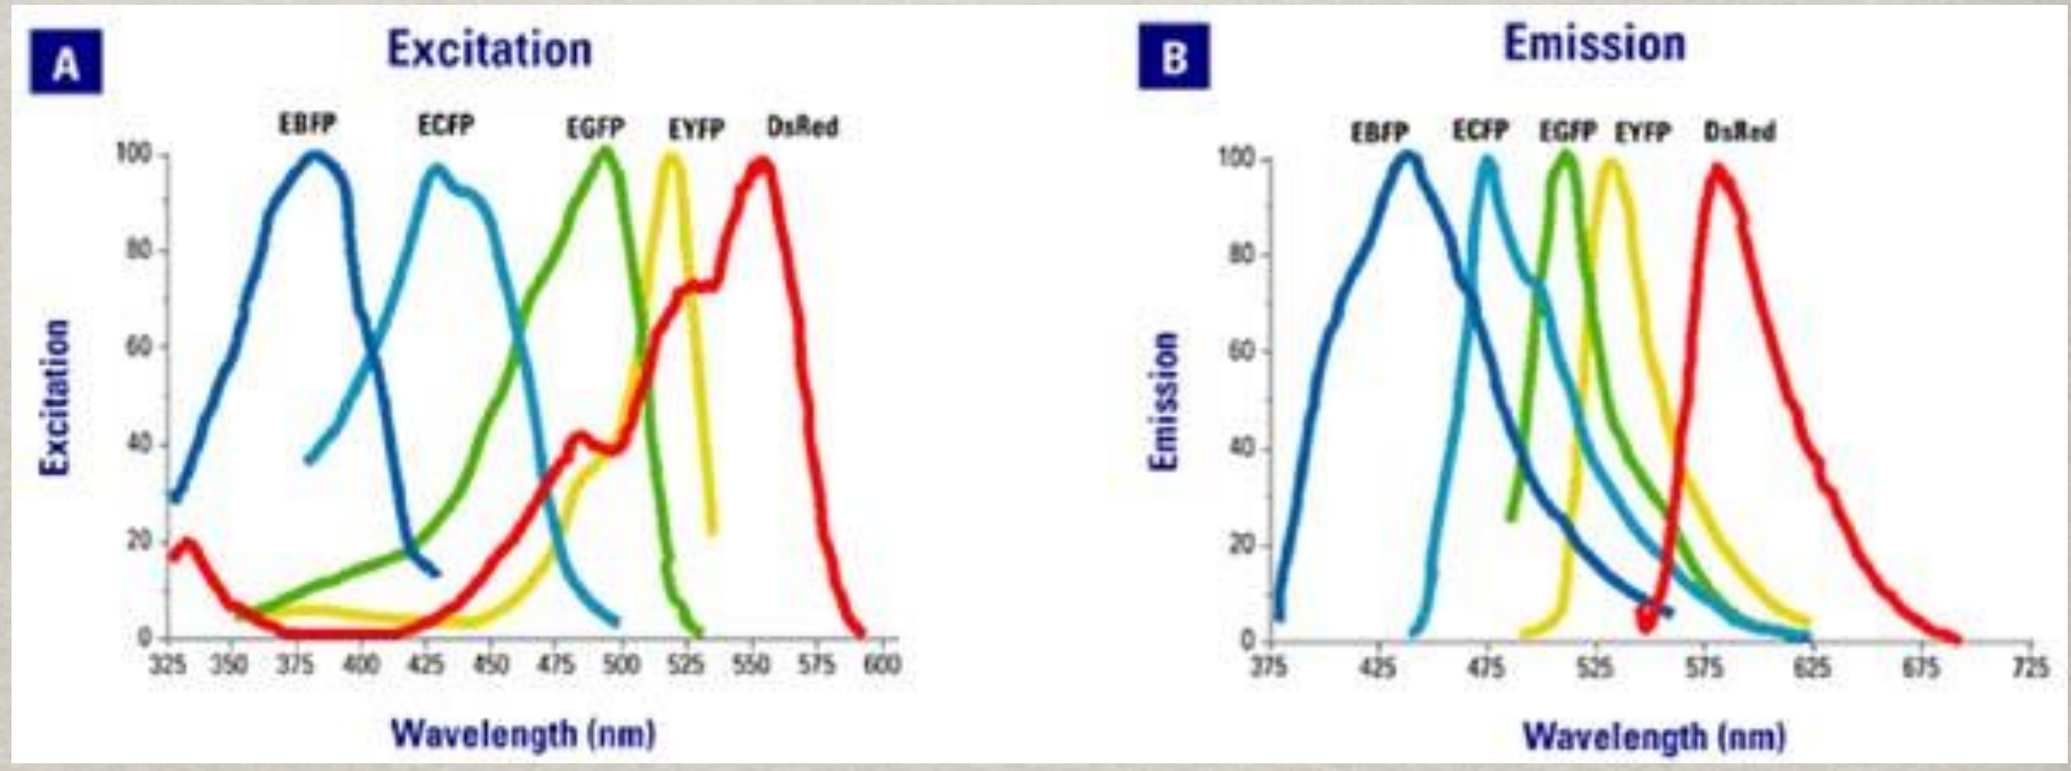

White Light provides All Wavelengths?

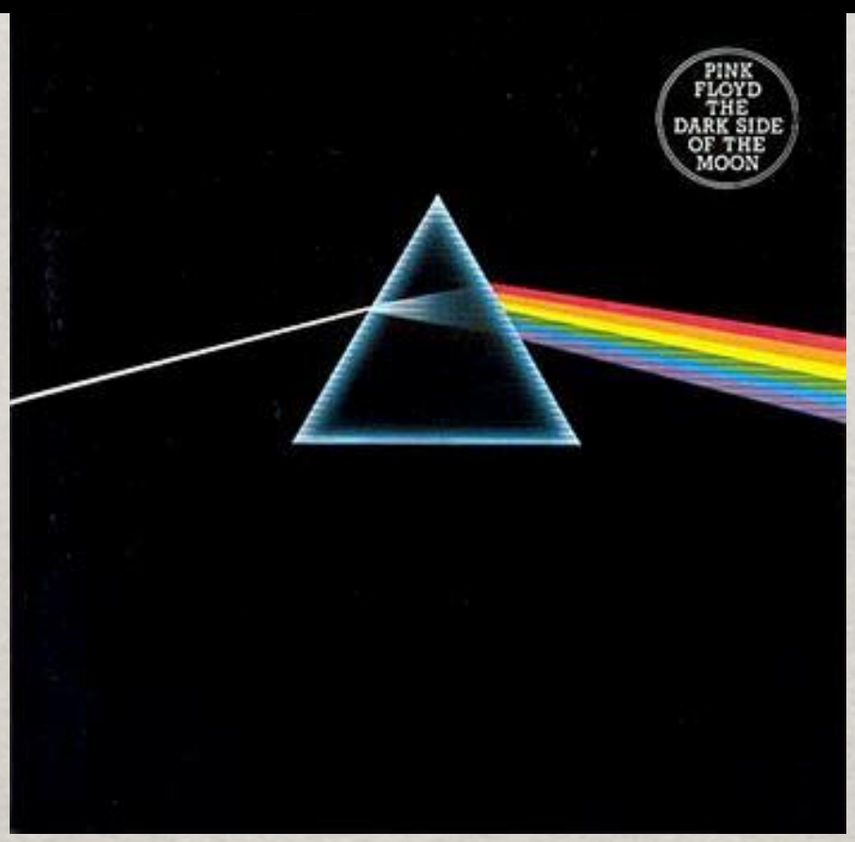

Spectra of White Florescent Light

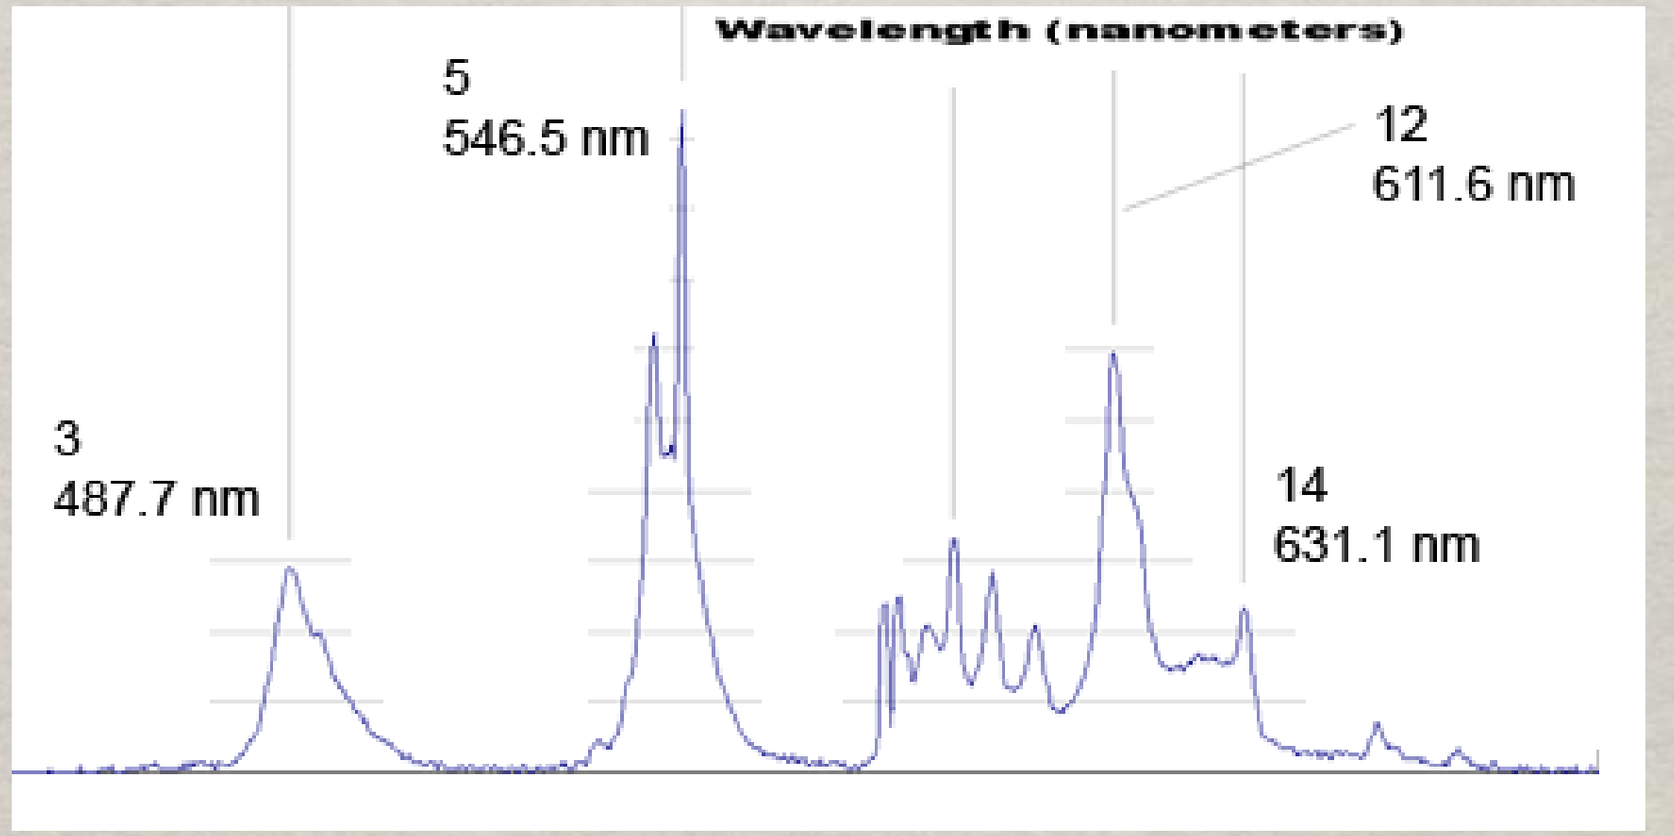

Spectrum of Light

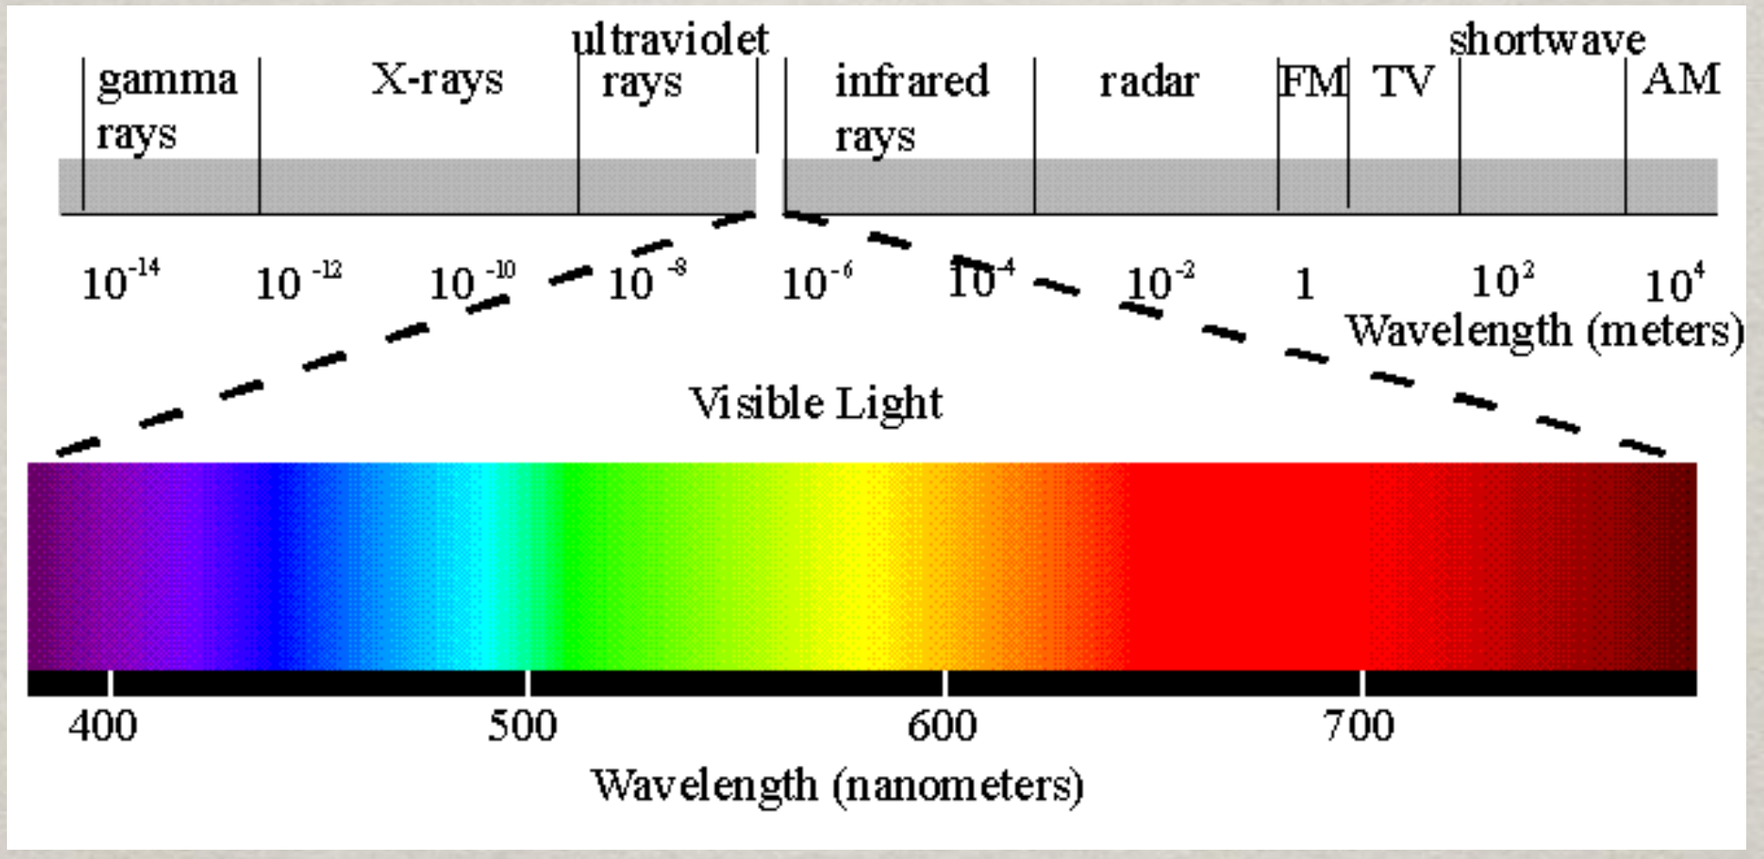

Common Sources In Microscopy

- Natural
- Filament
- Arc
- Solid State

Illumination Needs

- Spectral Requirements
- Directed
- Intense
- Even Illumination

Natural sources of light

Sunlight

Full Spectrum
Difficult to Harness
No Overnight Experiments

Fire

Spectrum Depends On Fuel
Difficult to Control
Avoid Wind!

Filament Lamps

Halogen Lamp Spectra

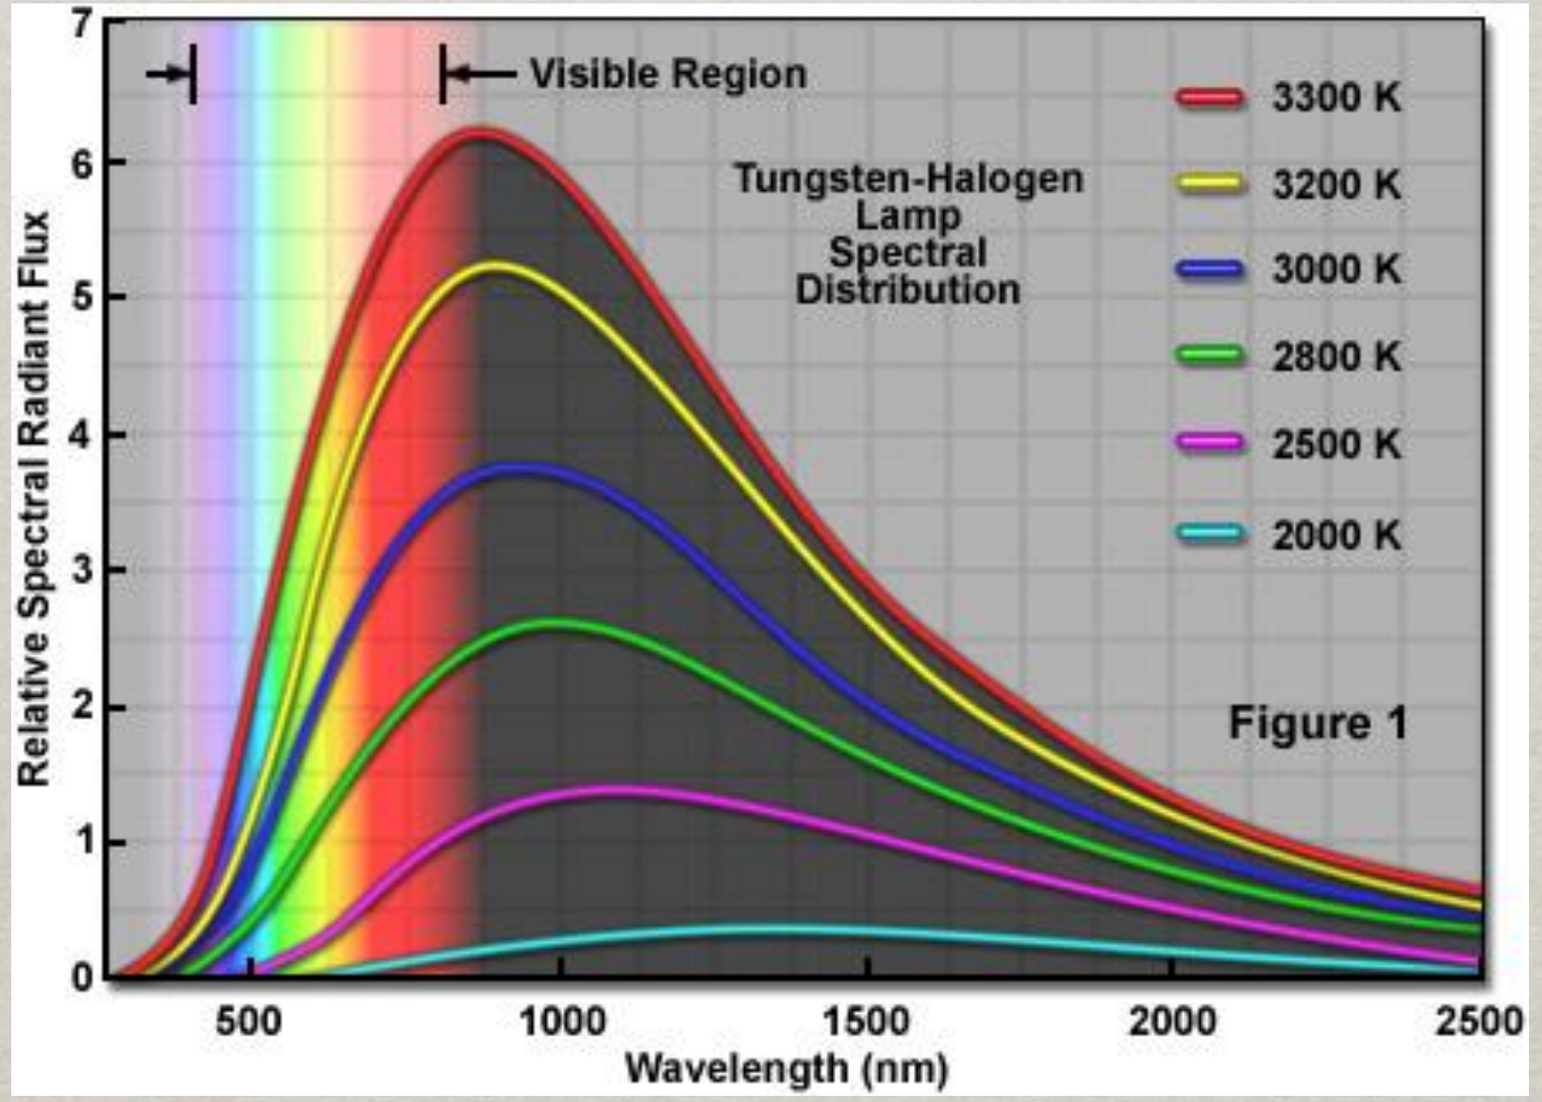

Typically Used for Brightfield Imaging Techniques

Arc Lamps

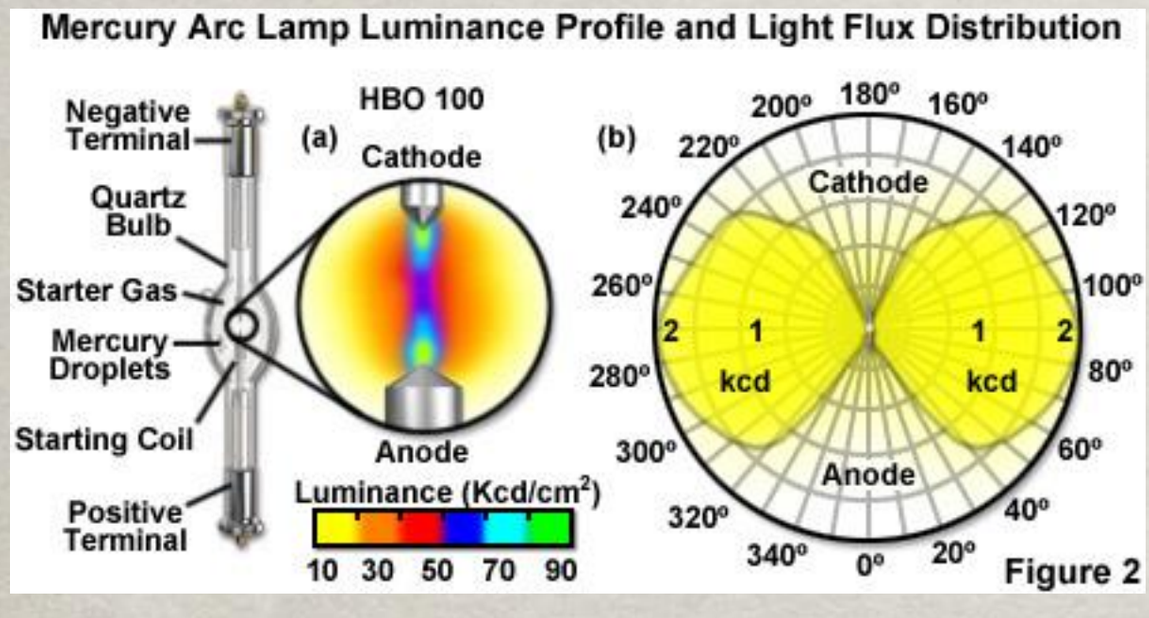

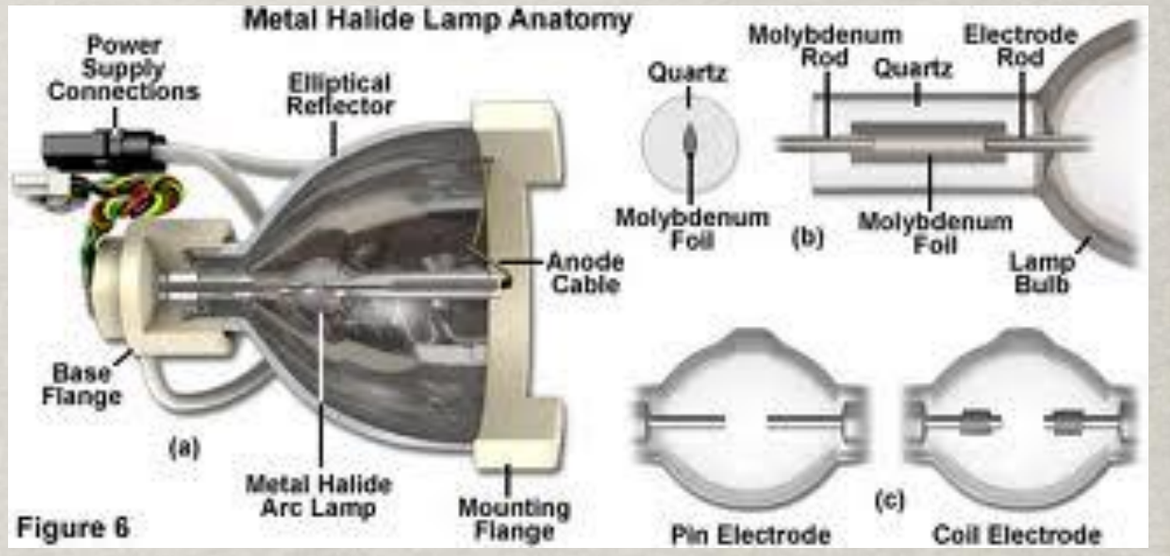

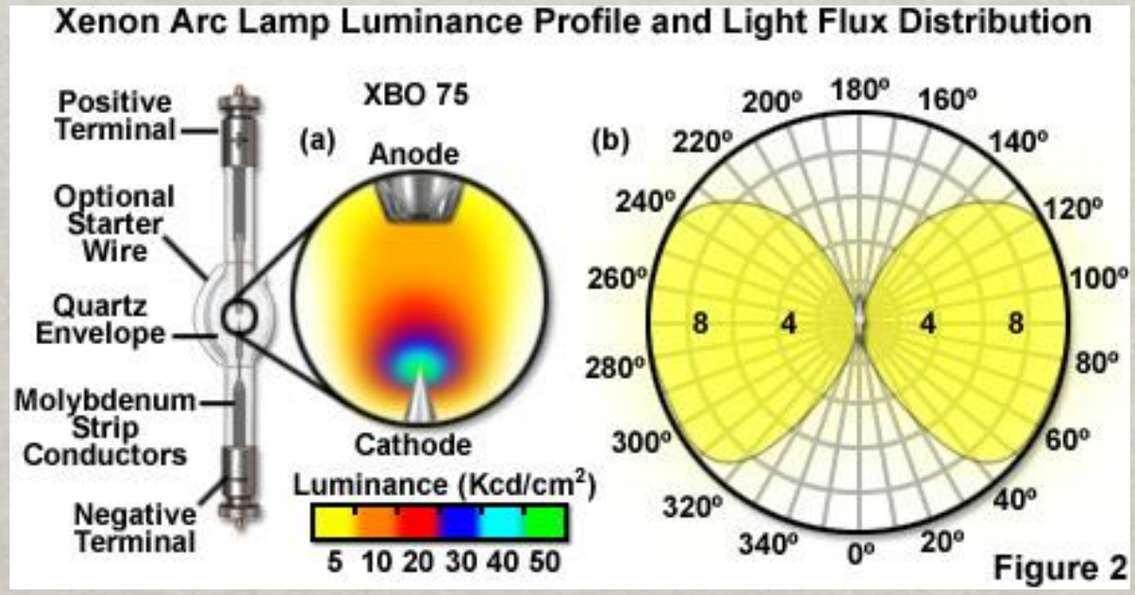

http://zeiss-campus.magnet.fsu.edu/

Peak levels are not comparable

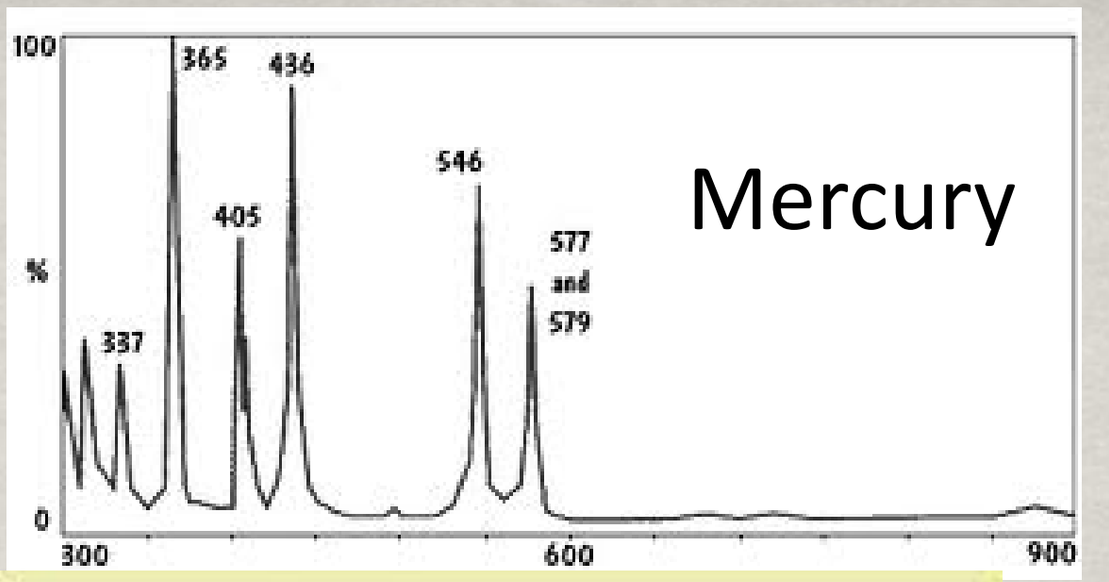

Mercury

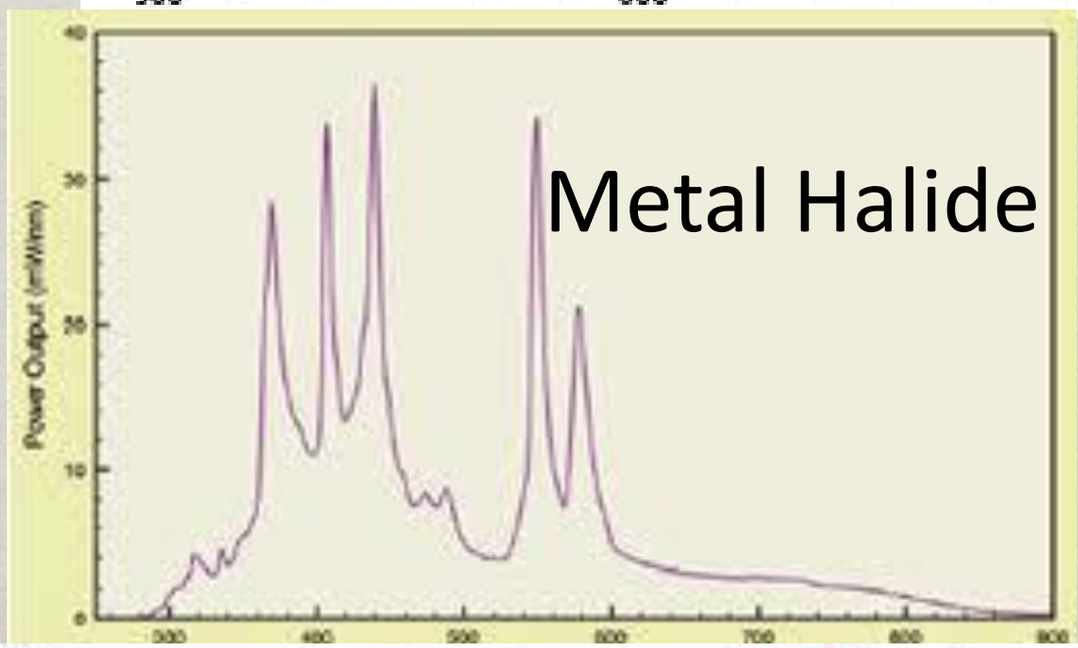

Metal Halide

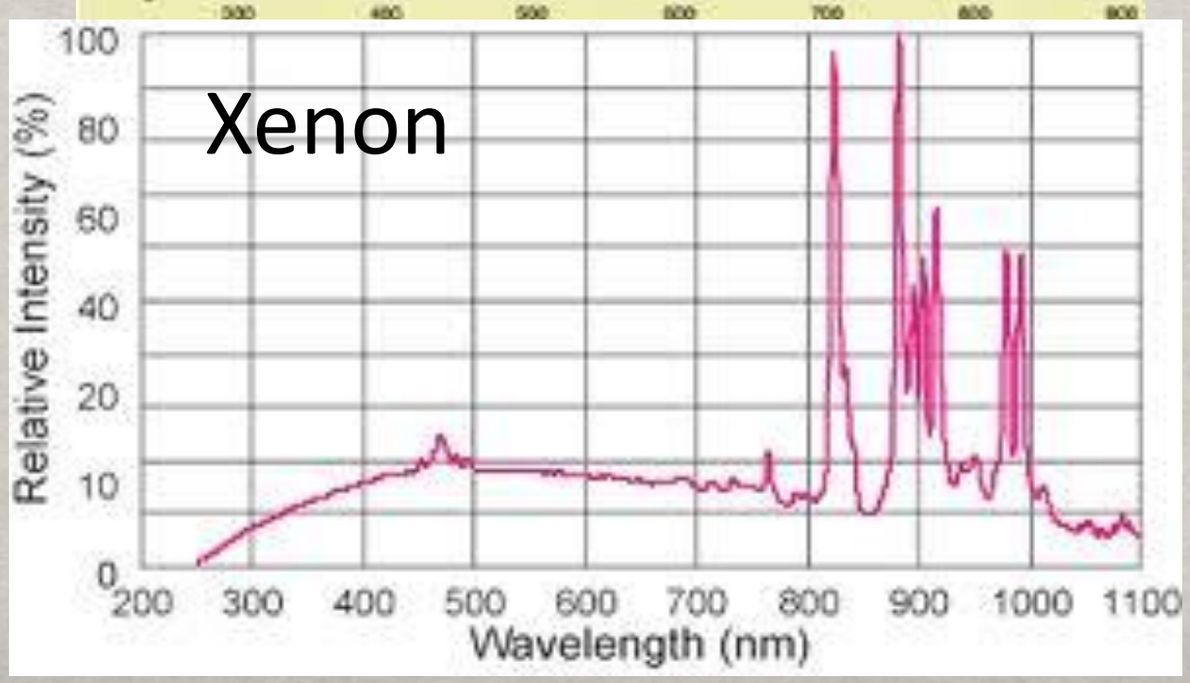

Xenon

Spectral Comparison

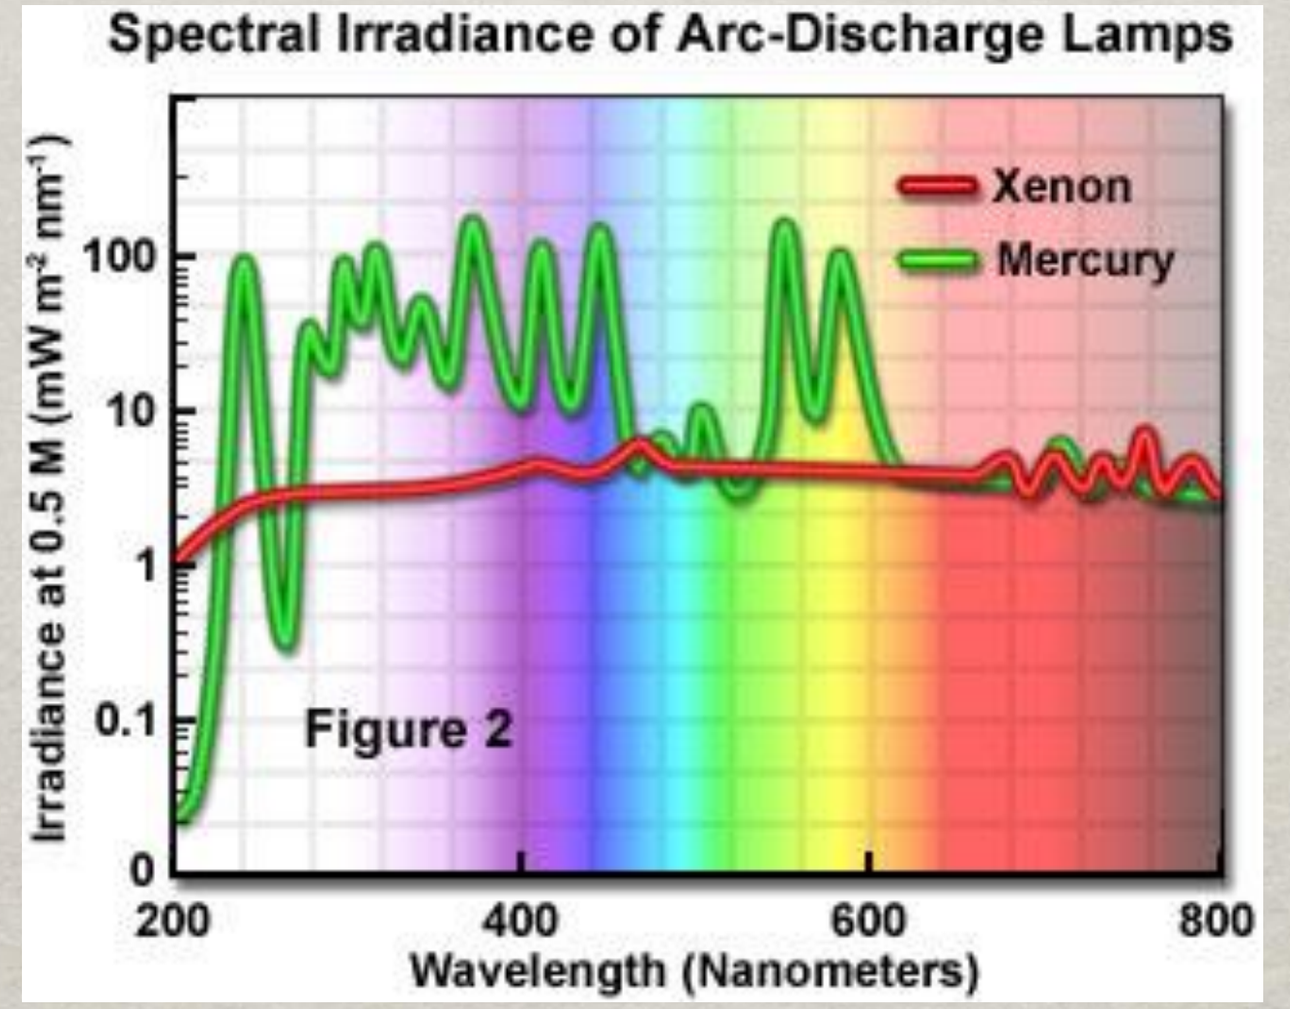

340nm and 380nm make Xenon ideal for Fura-2 imaging (Ca++)

Solid State Sources

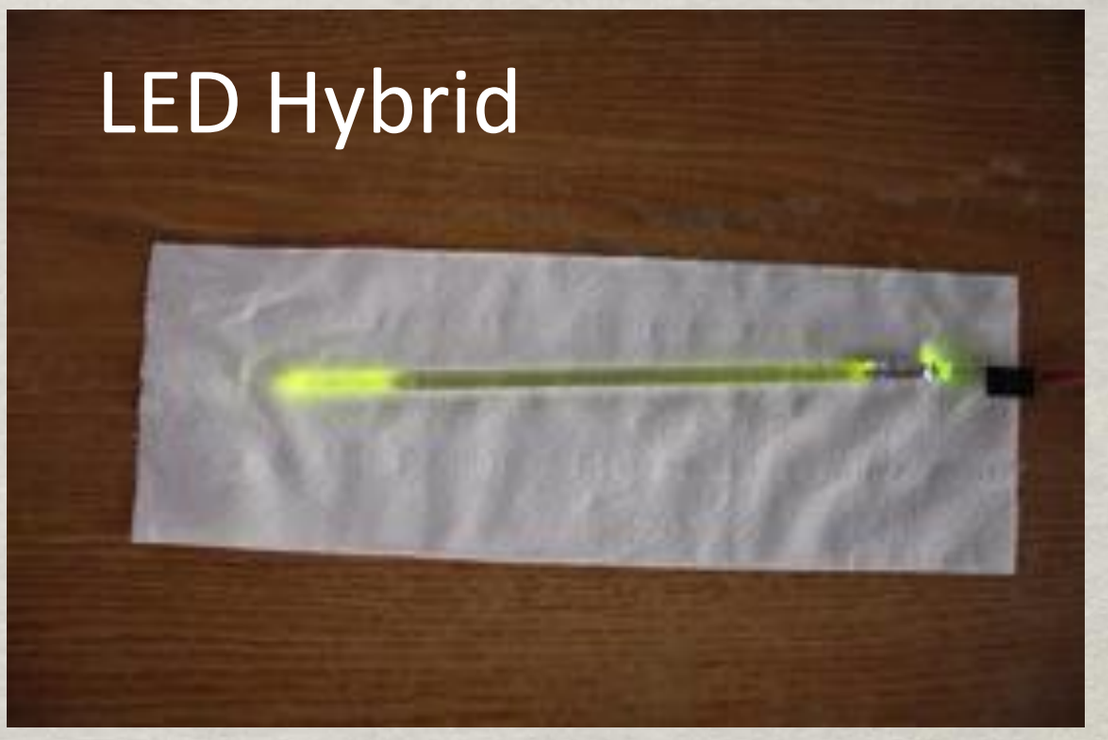

Light Emitting Diode

Don’t be [illegible] by the peak heights

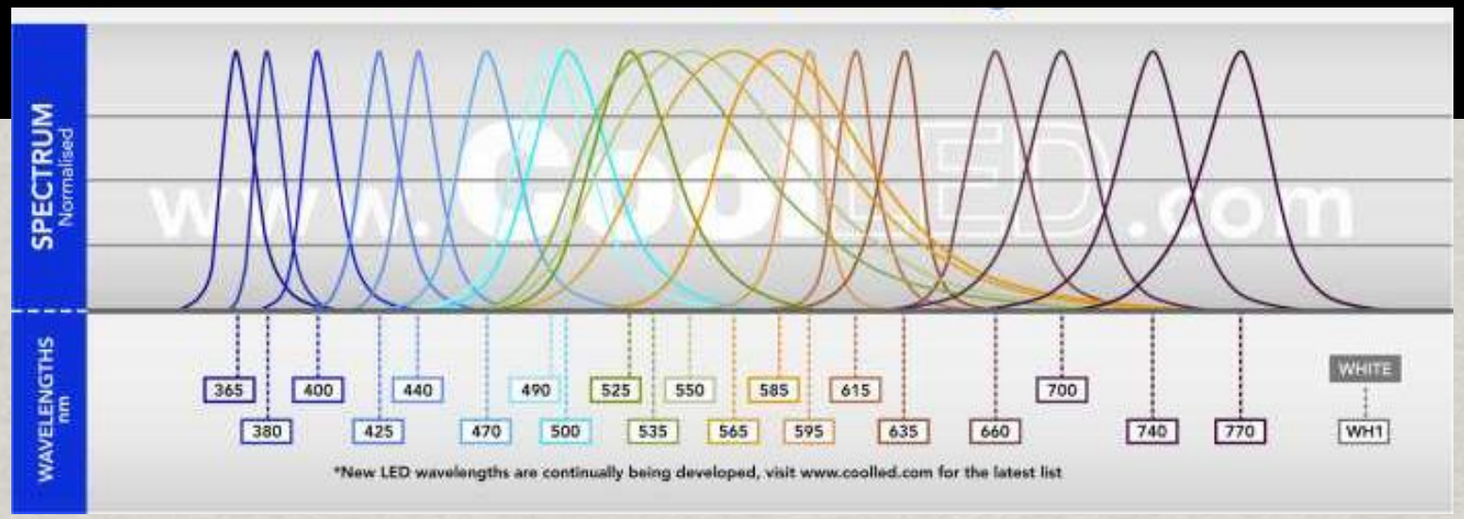

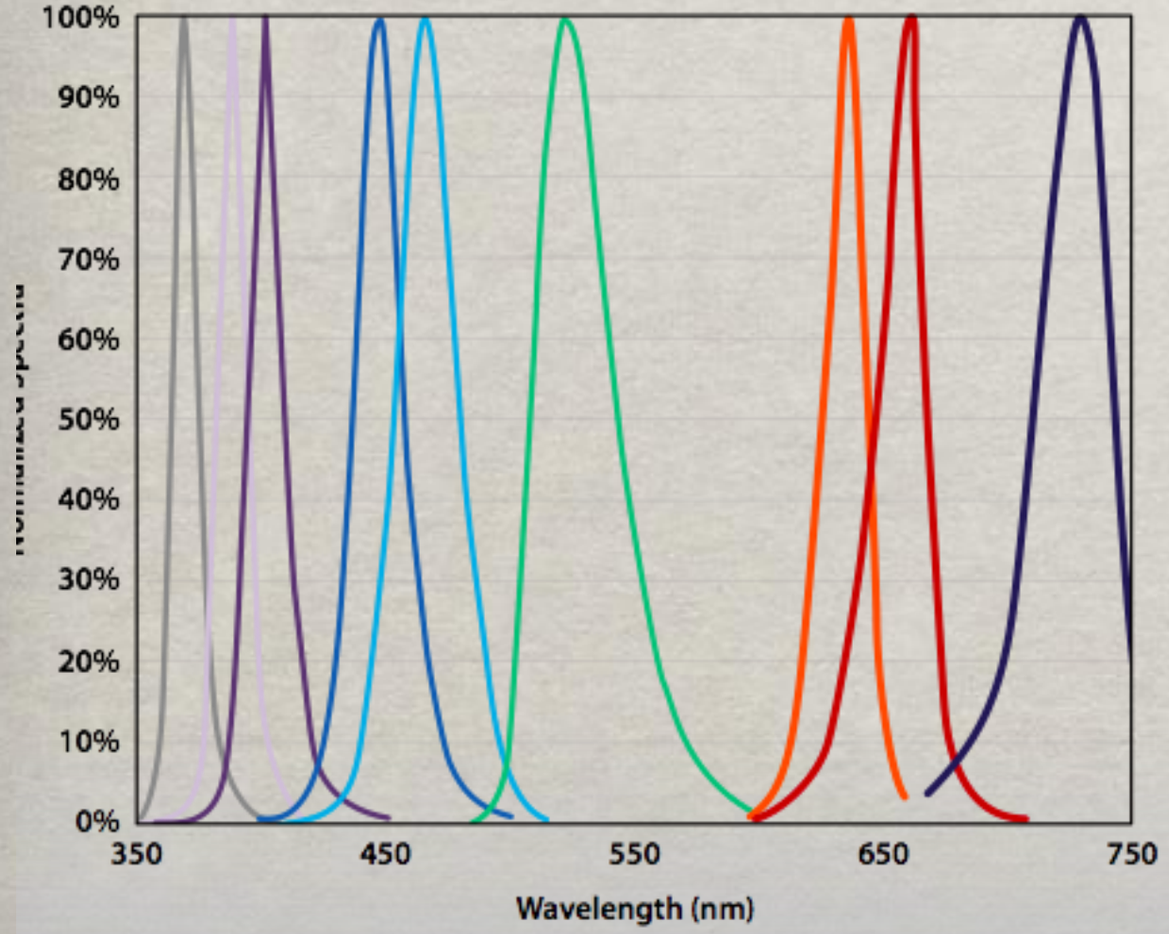

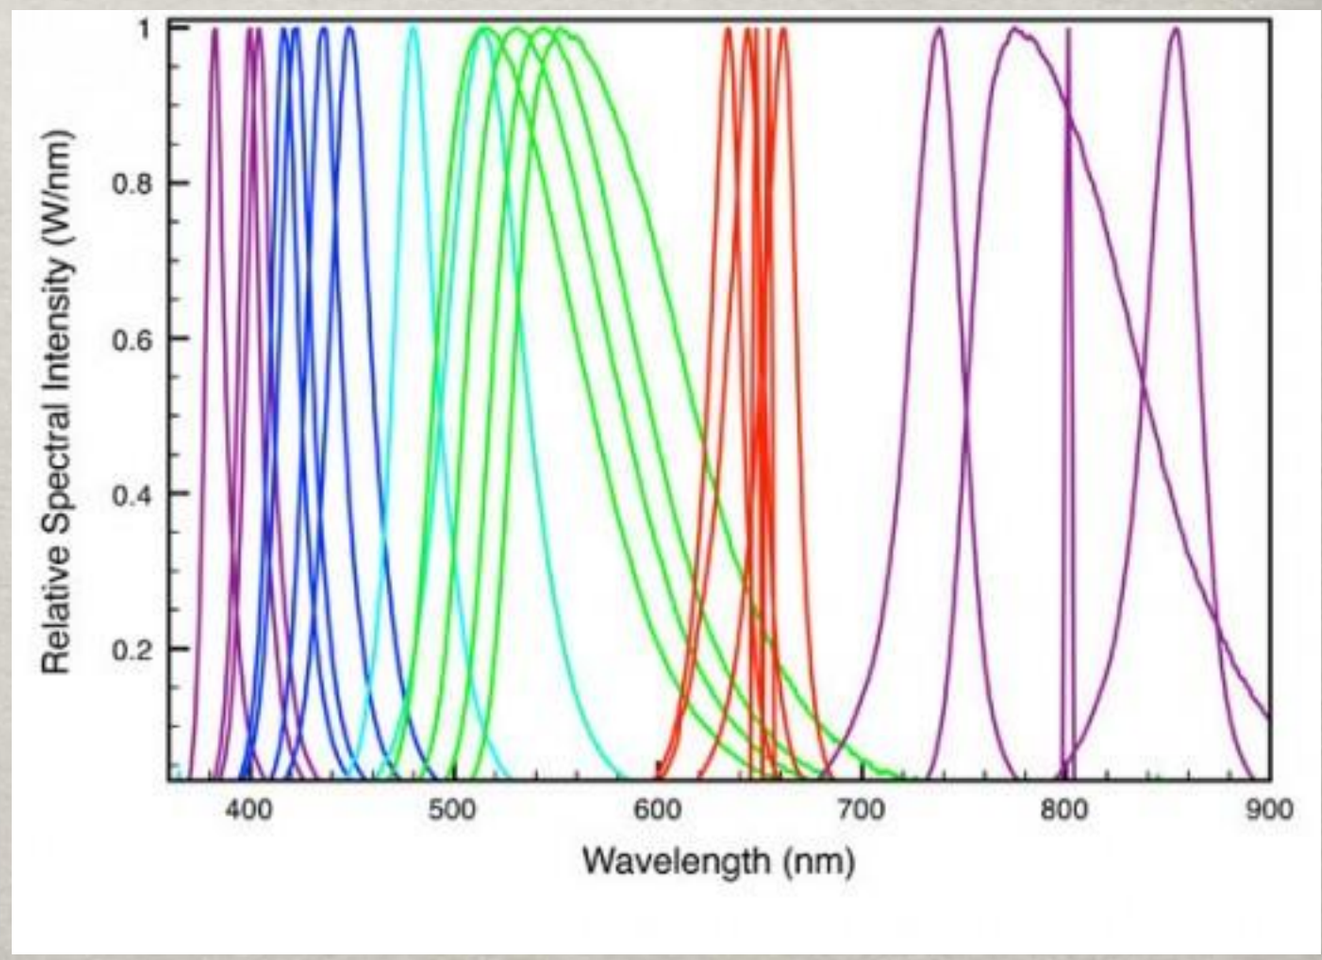

Light source Comparison

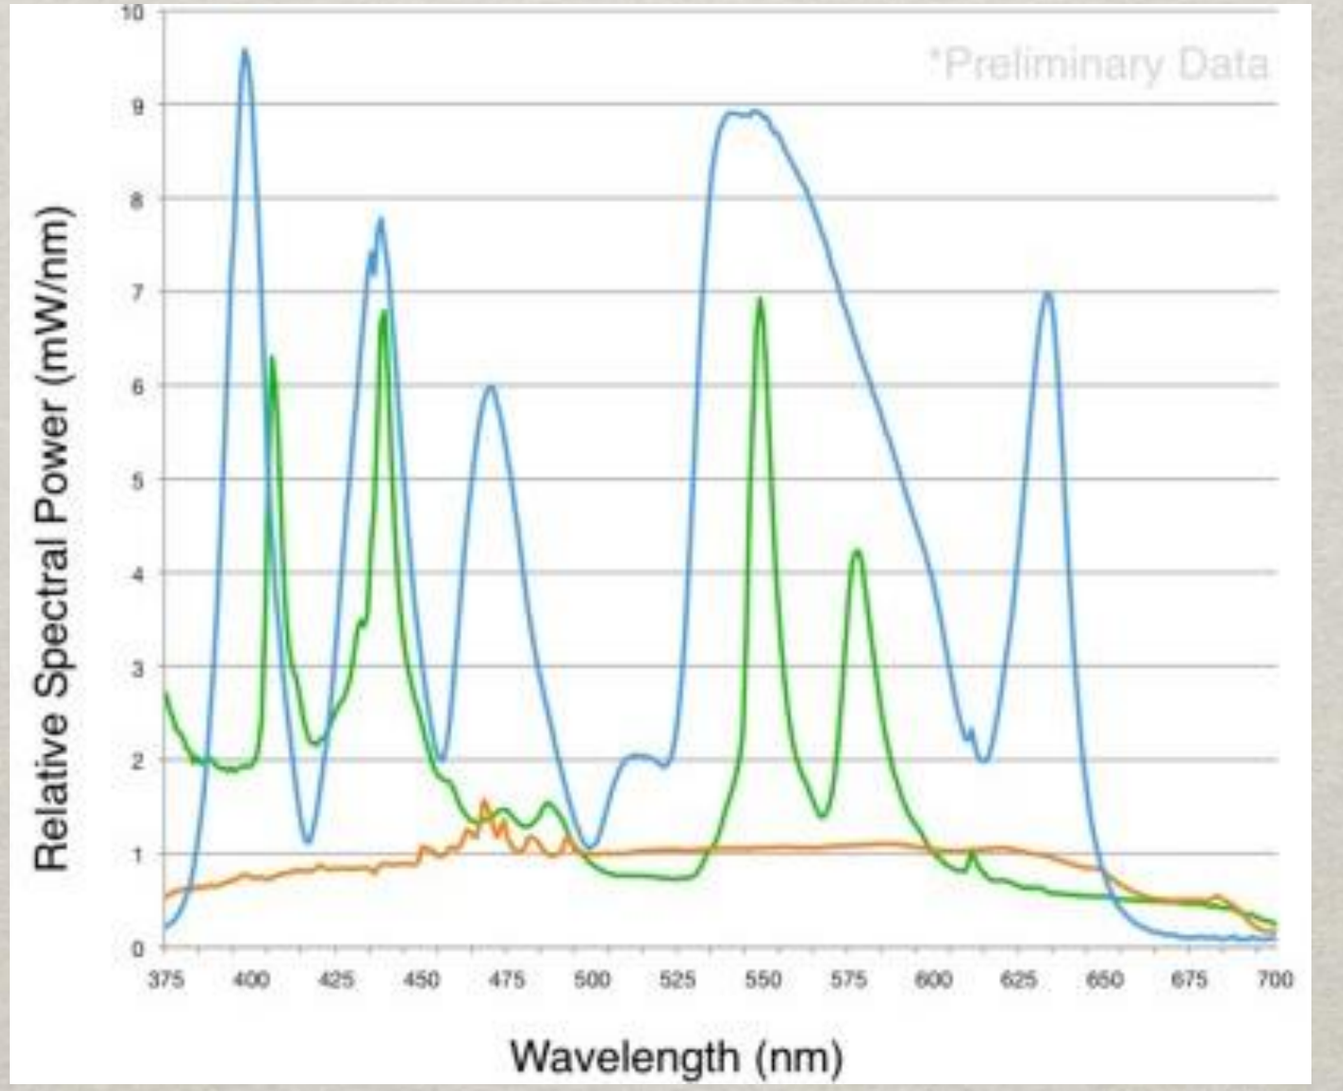

Filtered LED Source

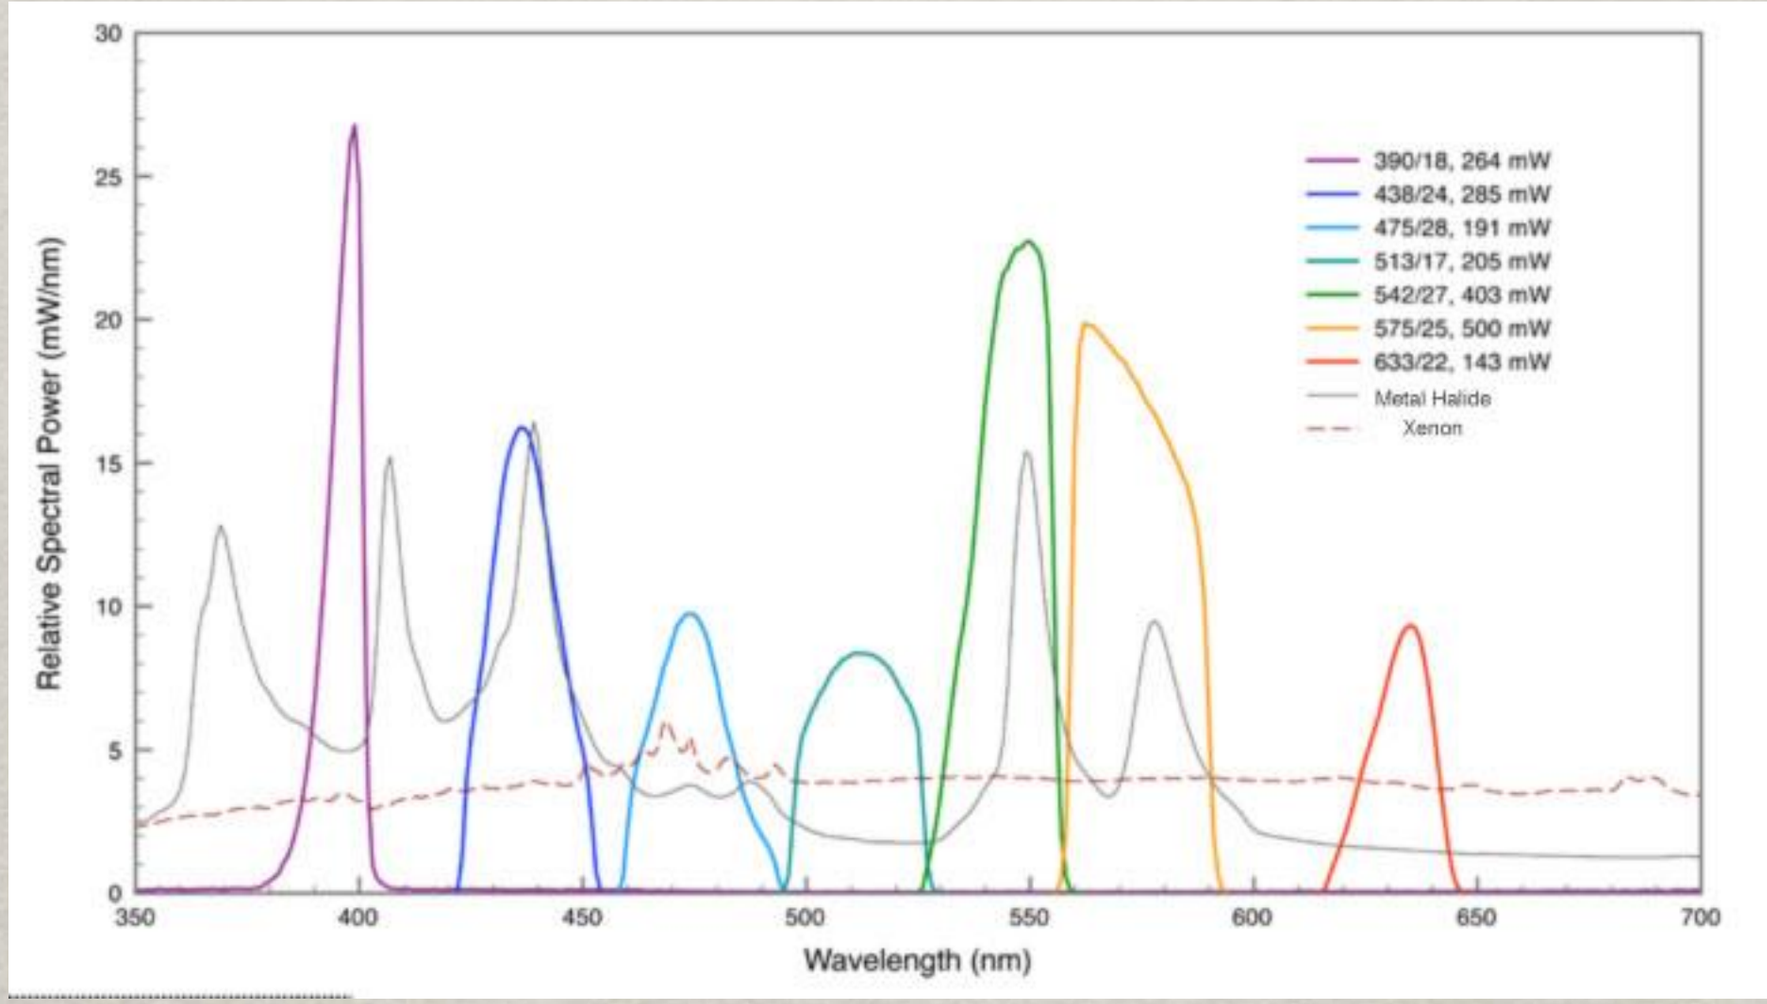

Light Source Comparison

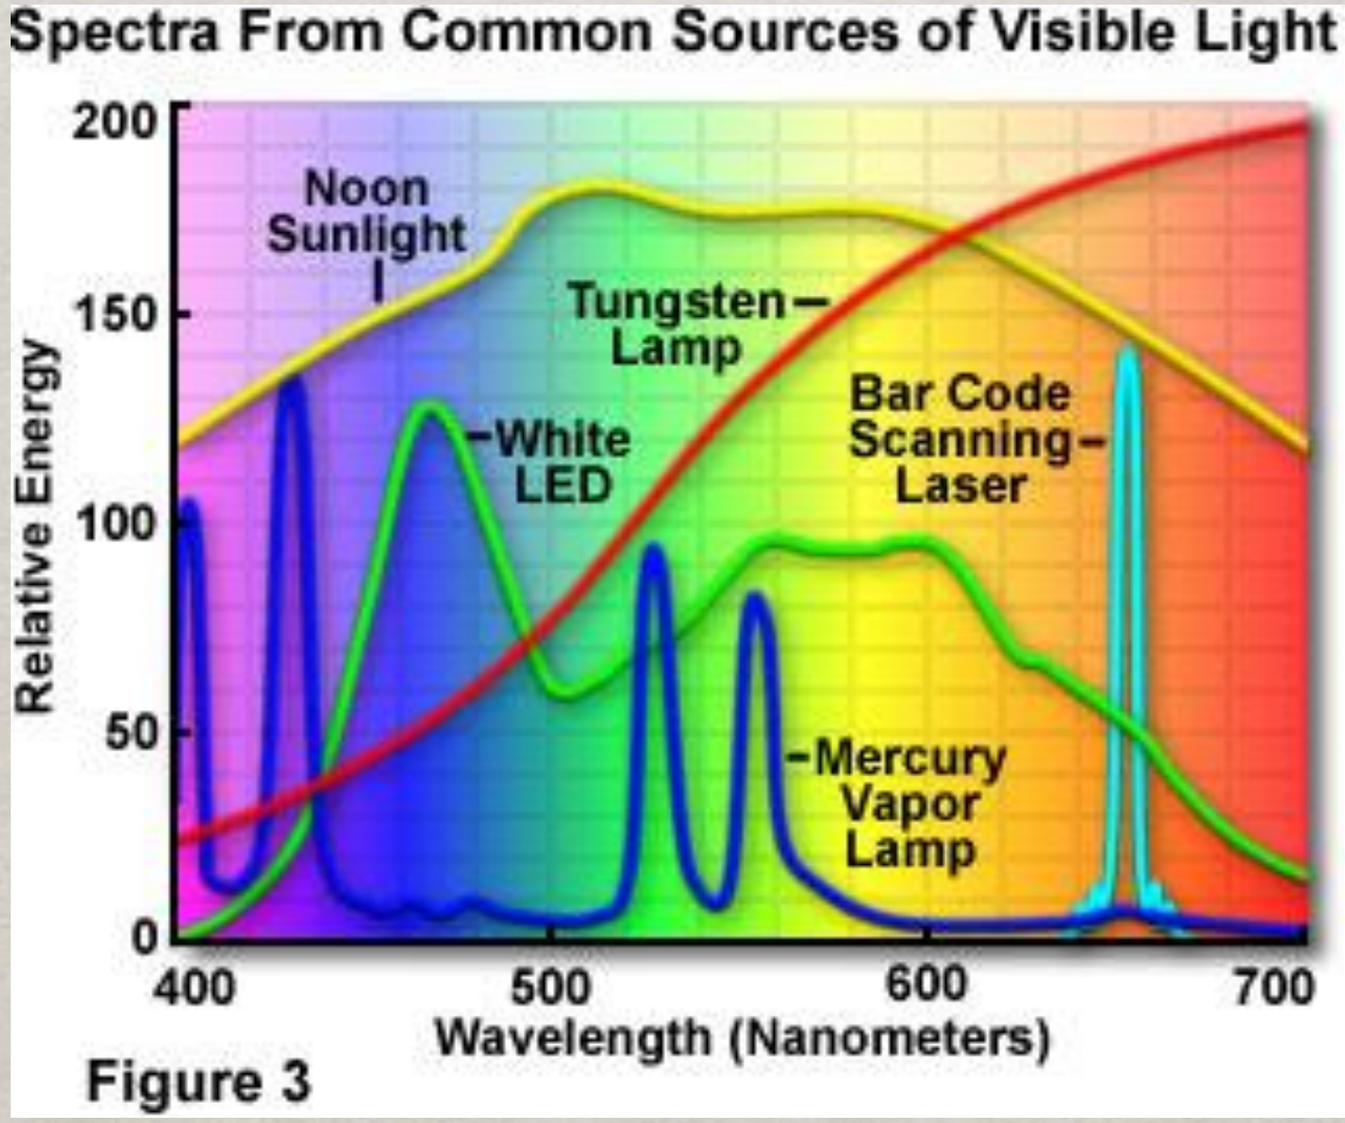

Figure 3

Common Fluorescence SOURCES

Source	Lifetime	Stability	Consumable Cost	Wavelength Range	Warm-up	Shutter/Switch Speed	Alignment	Time to 50% degradation (hr)	Flicker	Hazard	Heat	Green
Mercury	100	-	$200	UV - 600	30 min	External	+++	Varies	++++	++++	++++	NO
Metal Halide	2000	+	$600	350-600	5 min	External	-	200	++	+++	++++	NO
Xenon	1000	++	$600	340-1000	5 min	External	-	500	+	++++	++++	NO
LED	20000	++++	0	360-800	>1 min	5kHZ	-	20000	--	---	-	YES
Lasers	10000	++++	0	UV-IR	> 1 min	1MHz	-	10000	-	---	-	Yes

Thoughts on Light Source Comparisons

- Use Compatible Filters!!!
- Where does the measurement matter most?
- What is the unit of measure?
- What is the area of illumination?
- What is the hour number on the source?
- What is the cost of ownership?