


Introduction to Light Microscopy



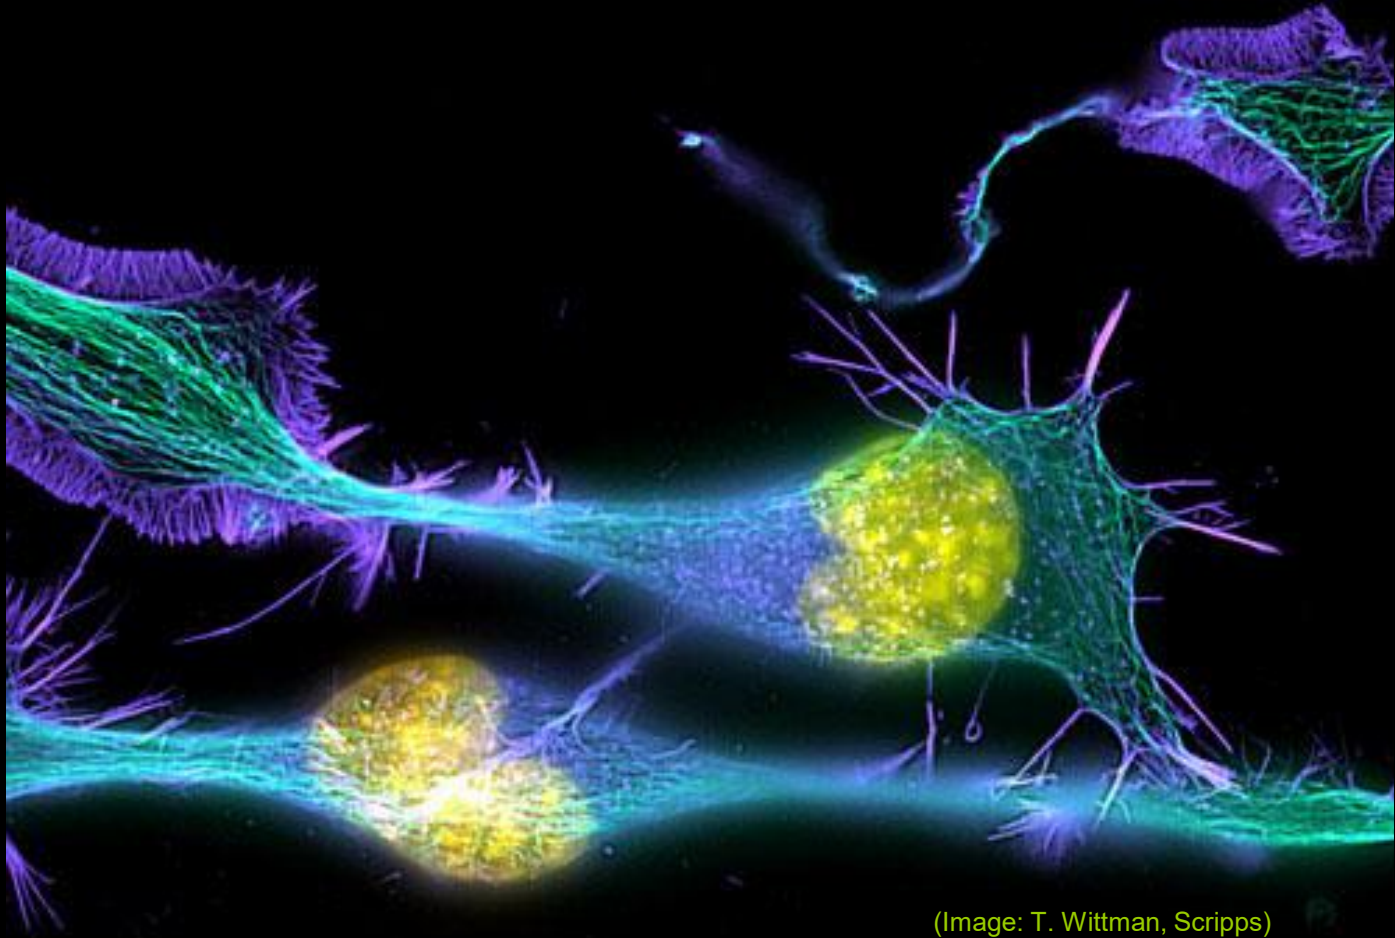


(Image: T. Wittman, Scripps)

The Light Microscope

- Four centuries of history
- Vibrant current development
- One of the most widely used research tools



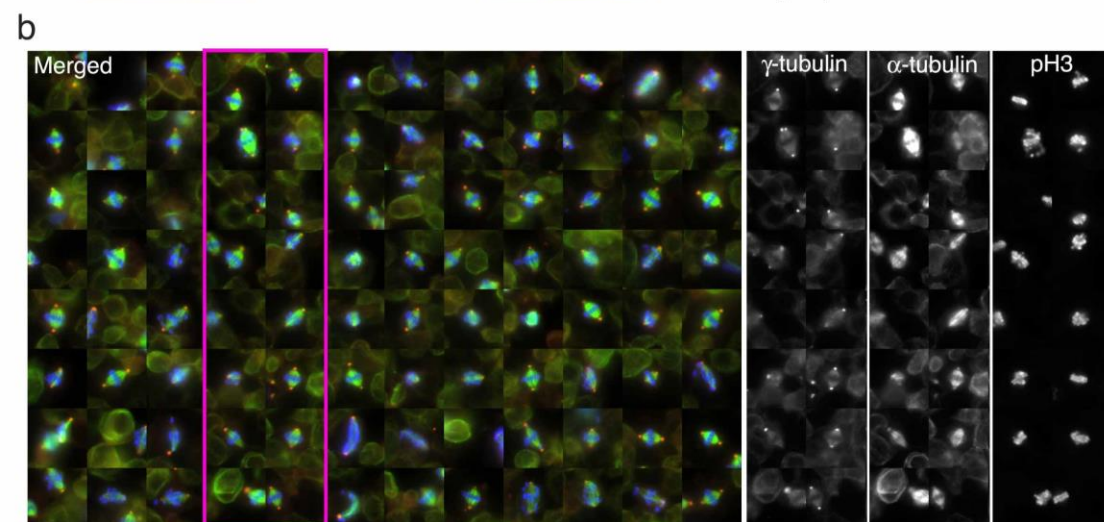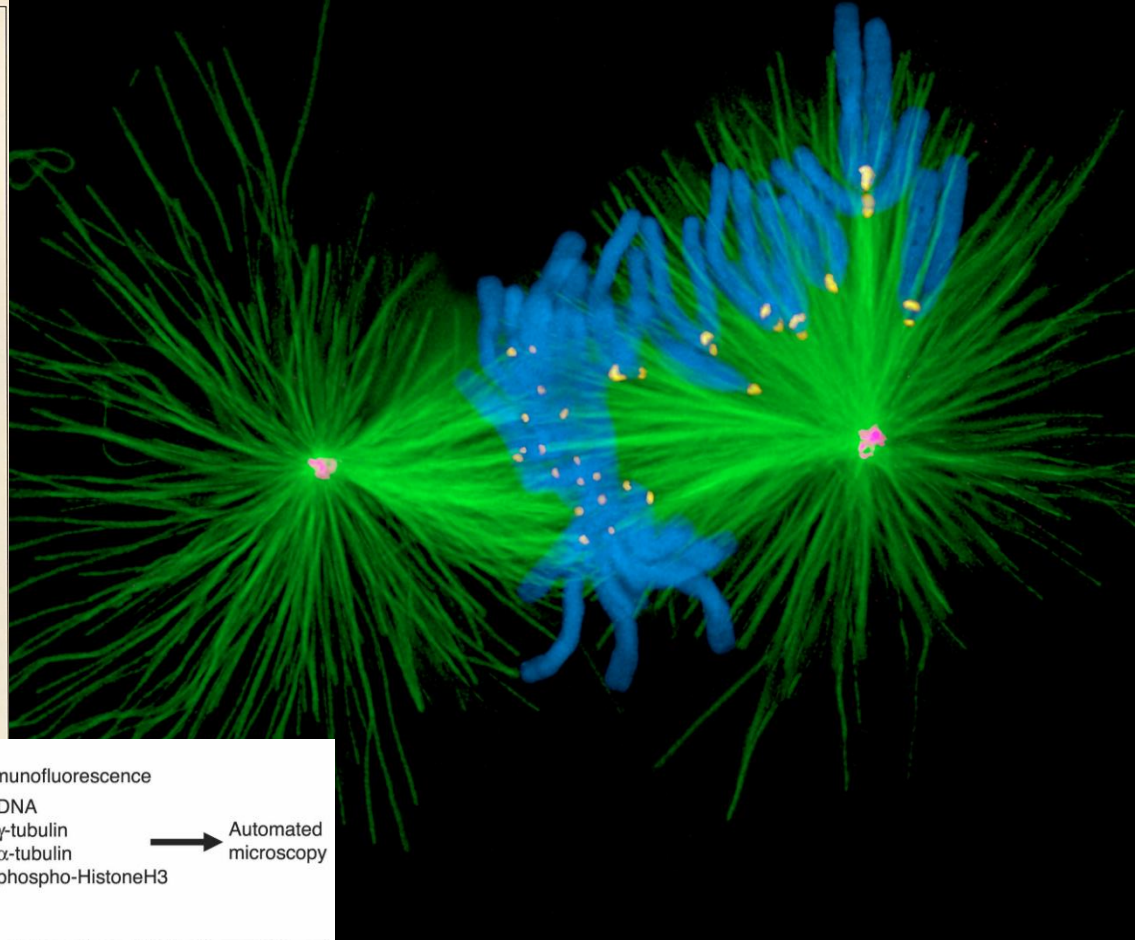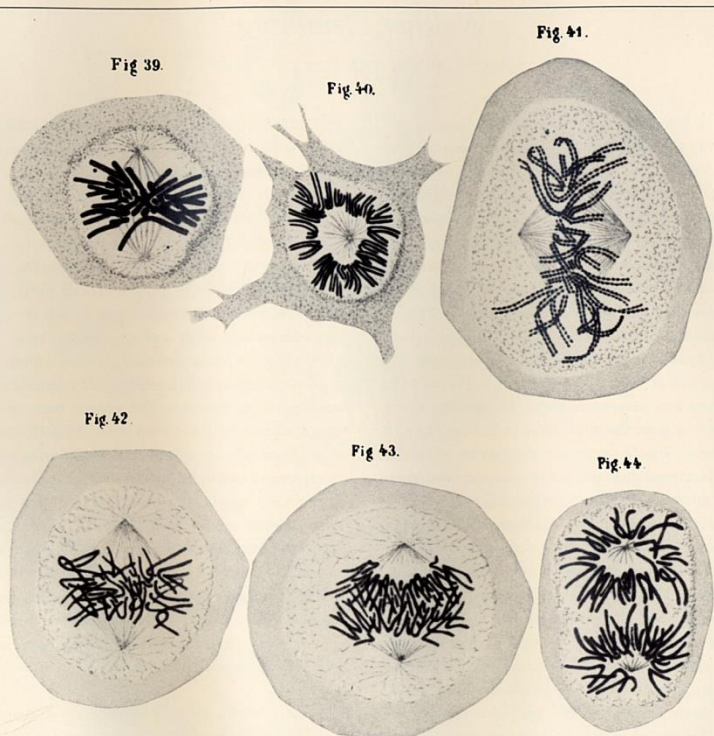

Major Imaging Functions of the Microscope

- Magnify
- Resolve features
- Generate Contrast
- Capture and Display Images

An Upright Epifluorescence Microscope


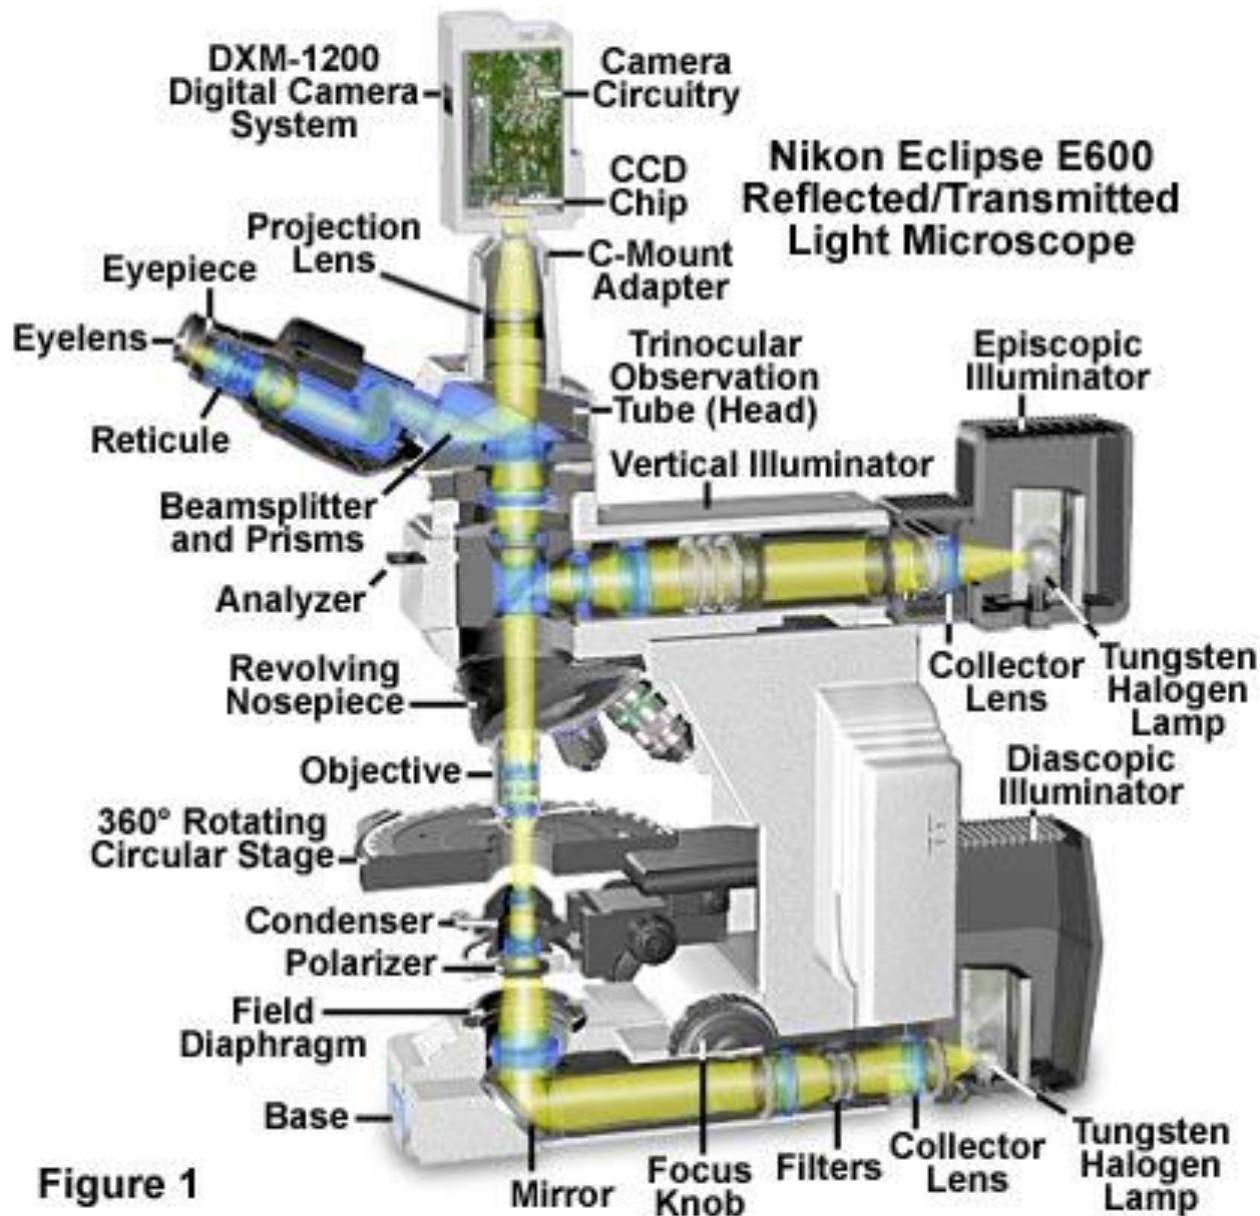


Figure 1

Light travels more slowly in matter

The speed ratio is the *Index of Refraction, n*

$$v = c/n$$

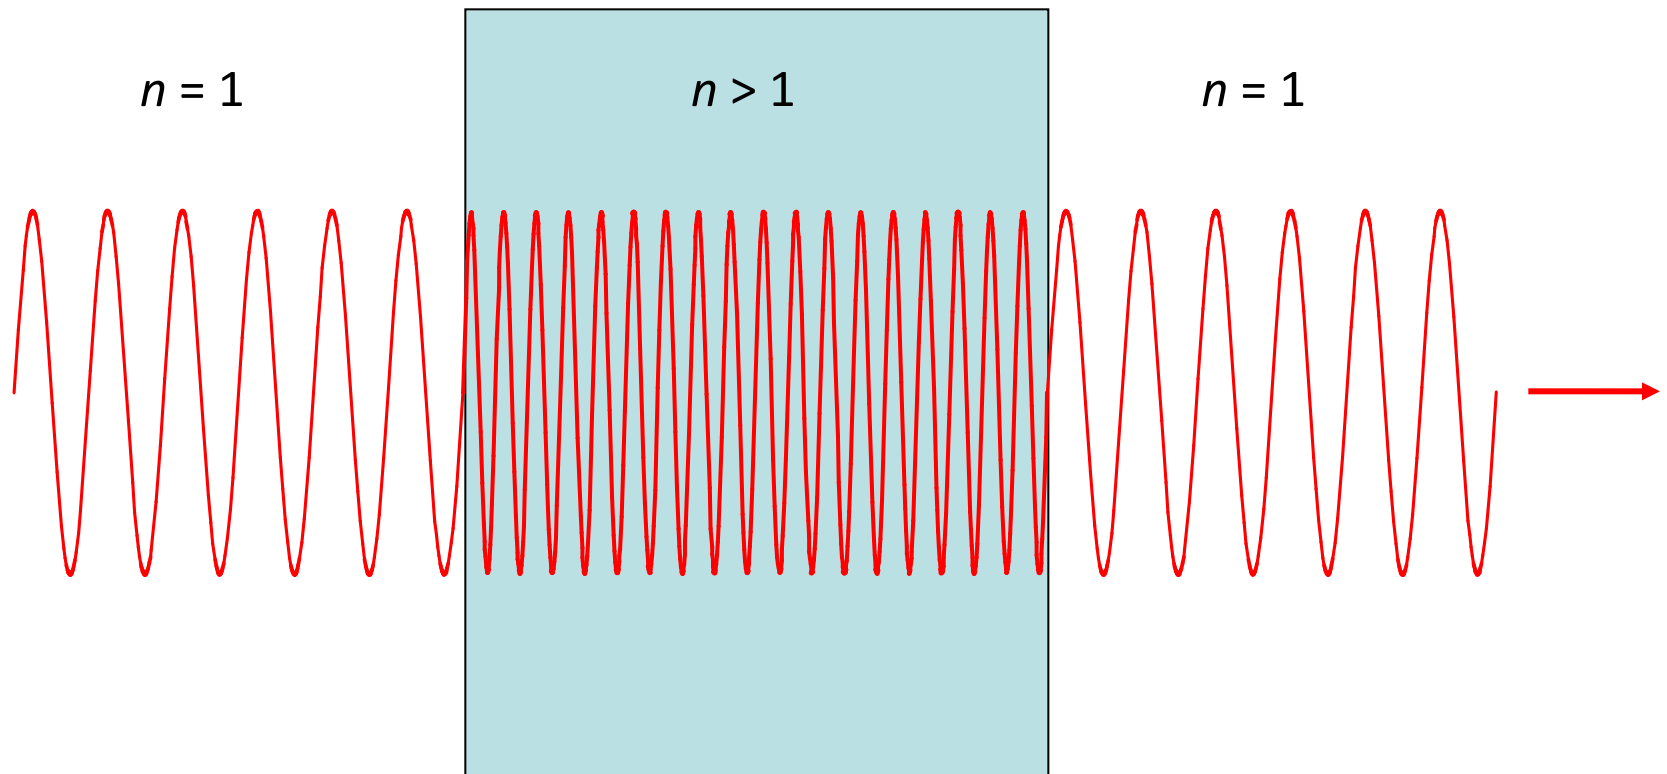


Refractive Index Examples

- Vacuum 1
- Air 1.0003
- Water 1.333
- Cytoplasm 1.35–1.38 ?
- Glycerol 1.475 (anhydrous)
- Immersion oil 1.515
- Fused silica 1.46
- Optical glasses 1.5–1.9
- Diamond 2.417


Depends on wavelength and temperature

Lenses work by refraction

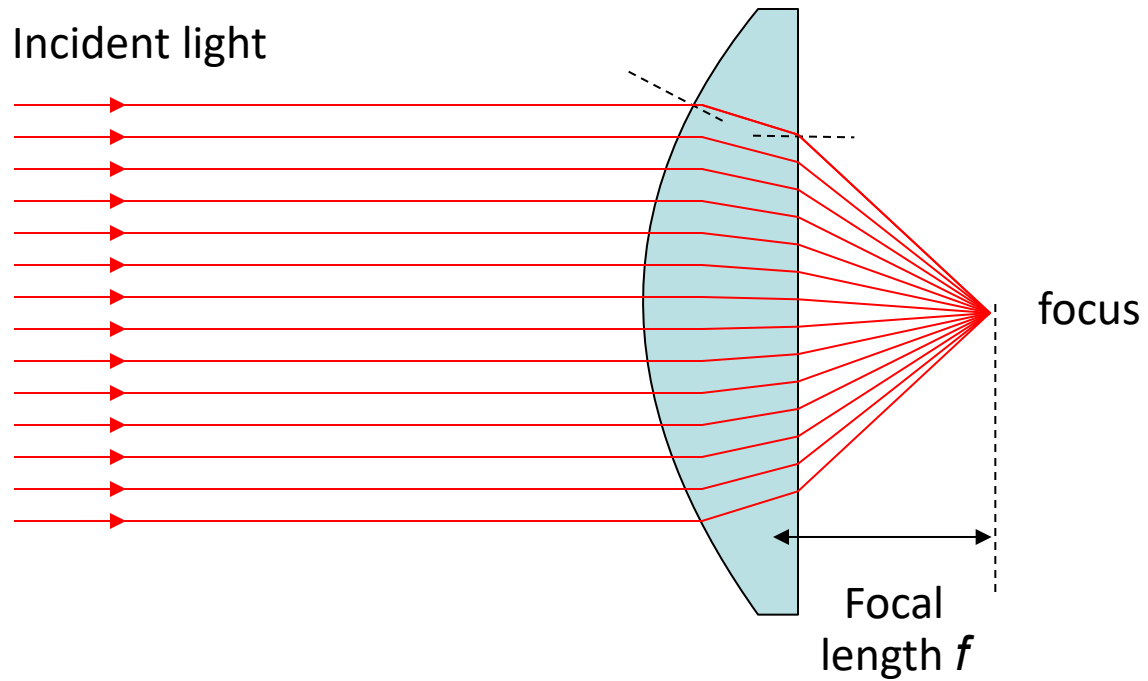

Finite vs. Infinite Conjugate Imaging

- Finite conjugate imaging (older objectives)

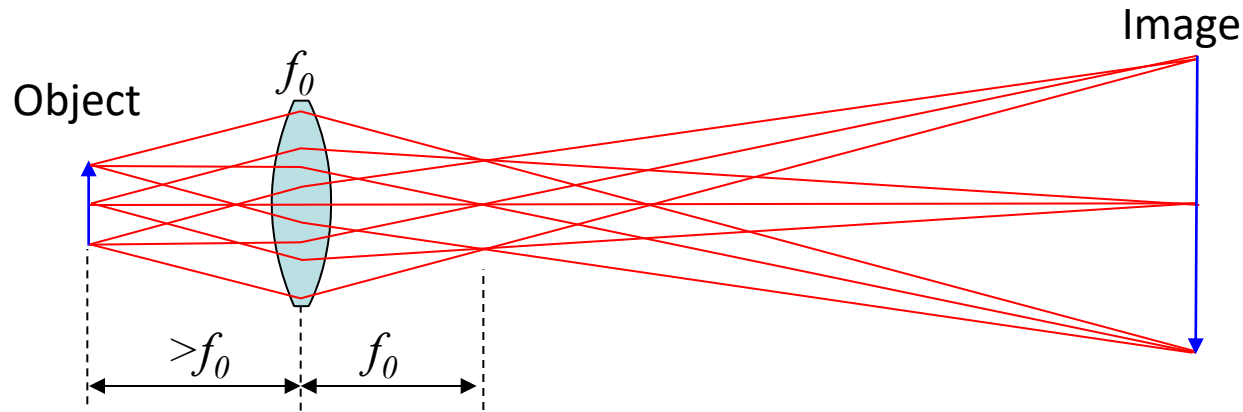

- Infinite conjugate imaging (modern objectives).


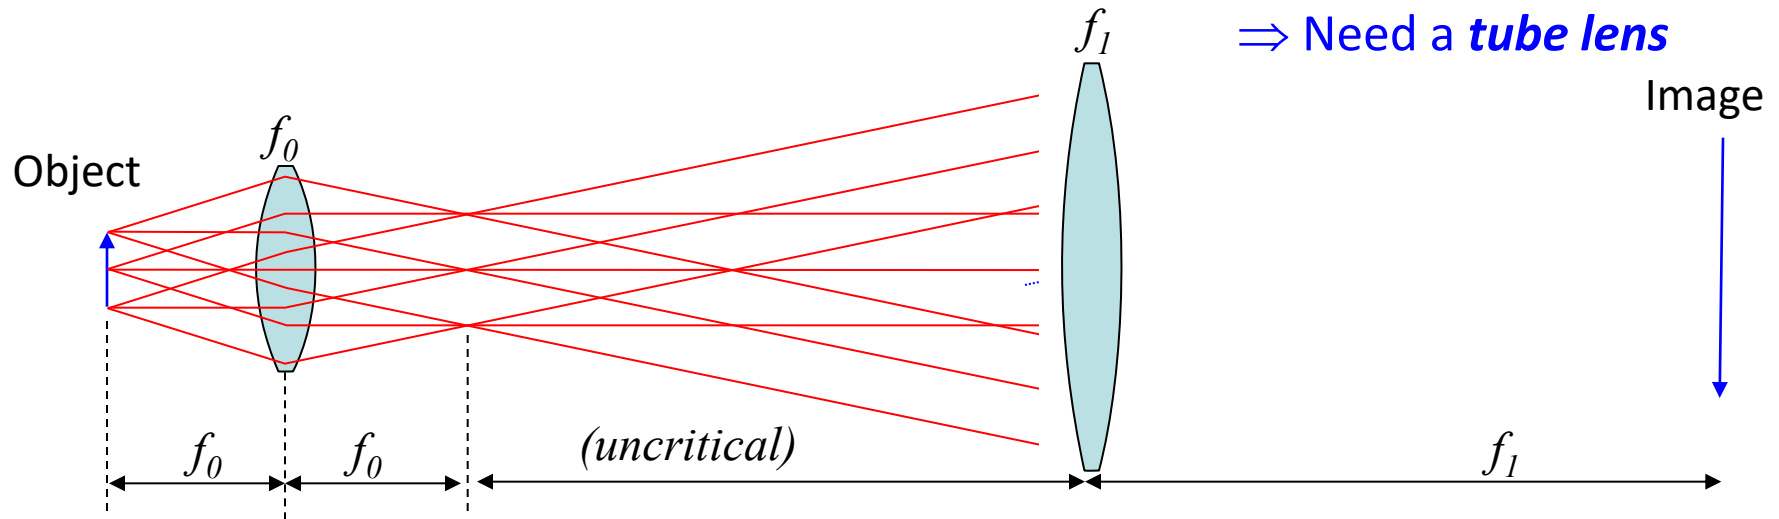


Image at infinity
 $\Rightarrow$ Need a **tube lens**


Magnification: $M = \frac{f_1}{f_o}$

Back focal plane

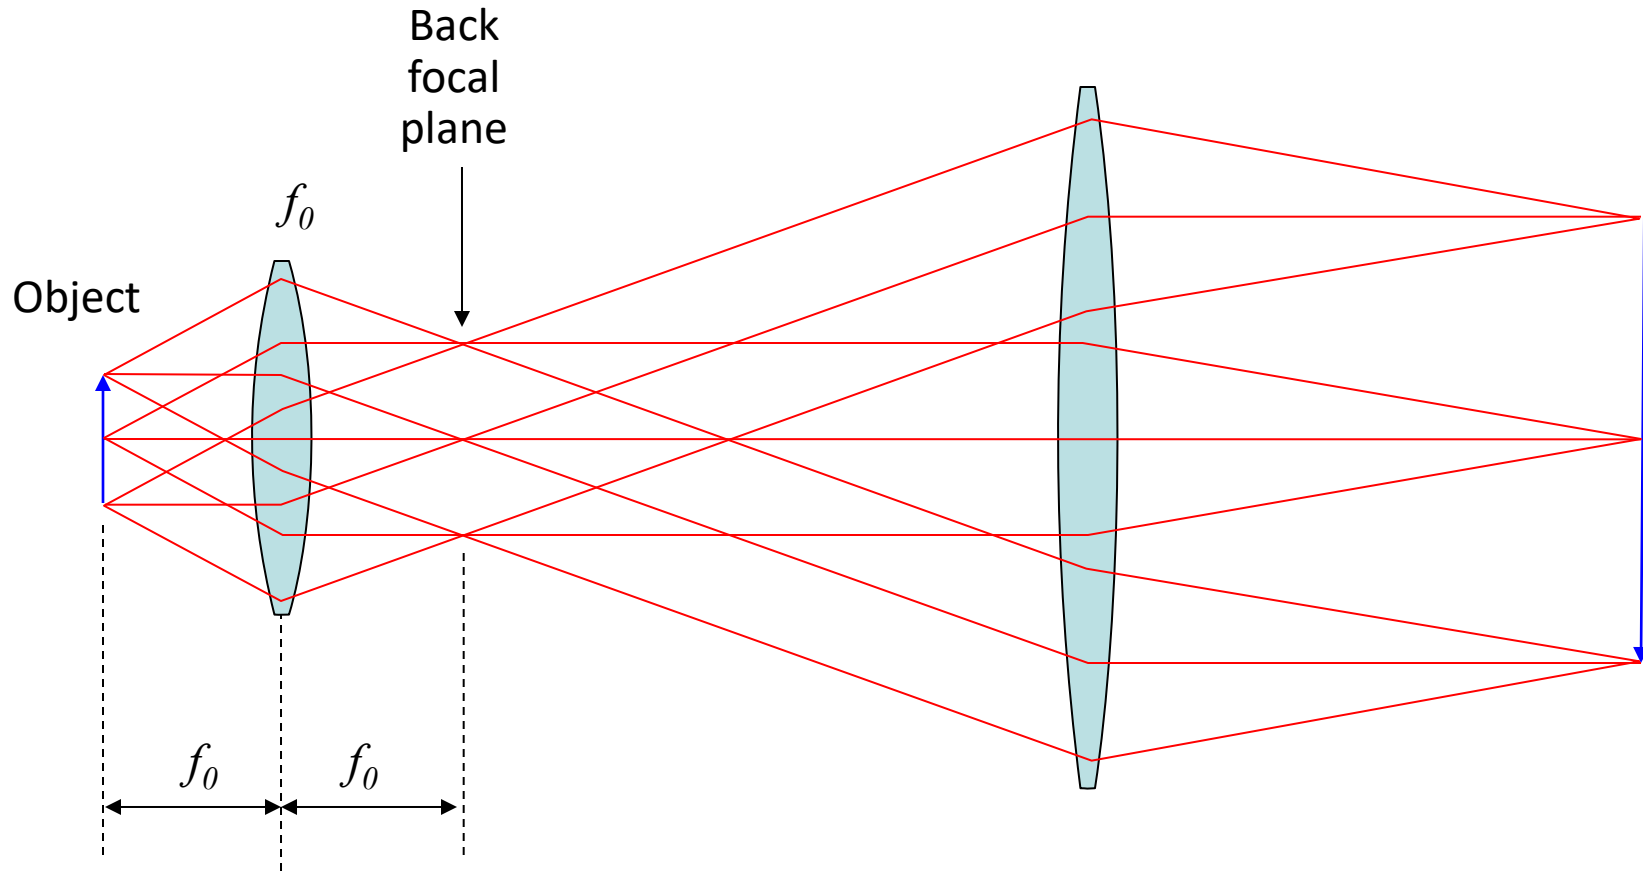


Rays that leave the object with the same angle meet in the objective's *back focal plane*


The Compound Microscope

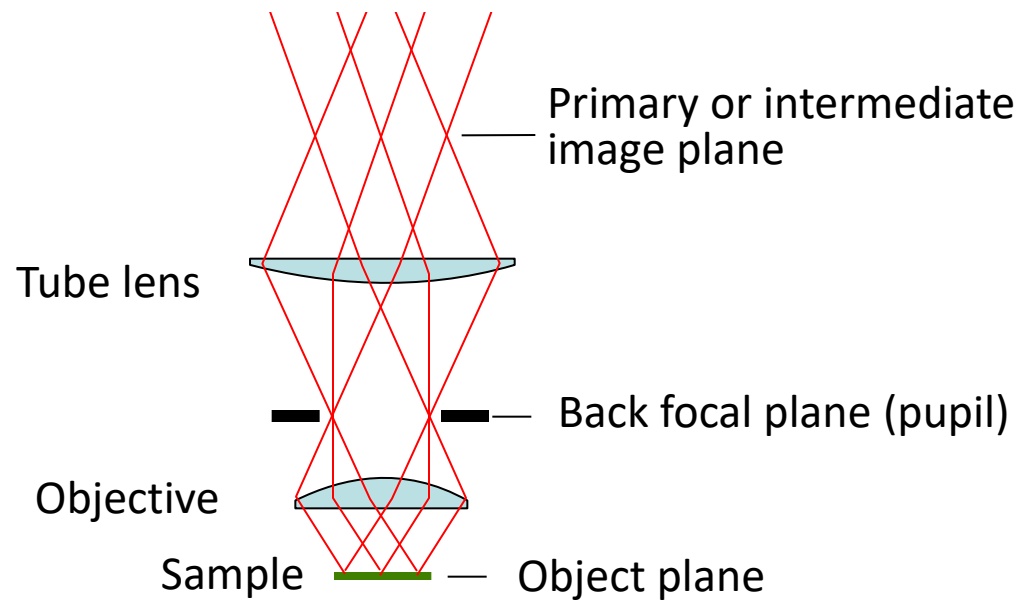


The Compound Microscope

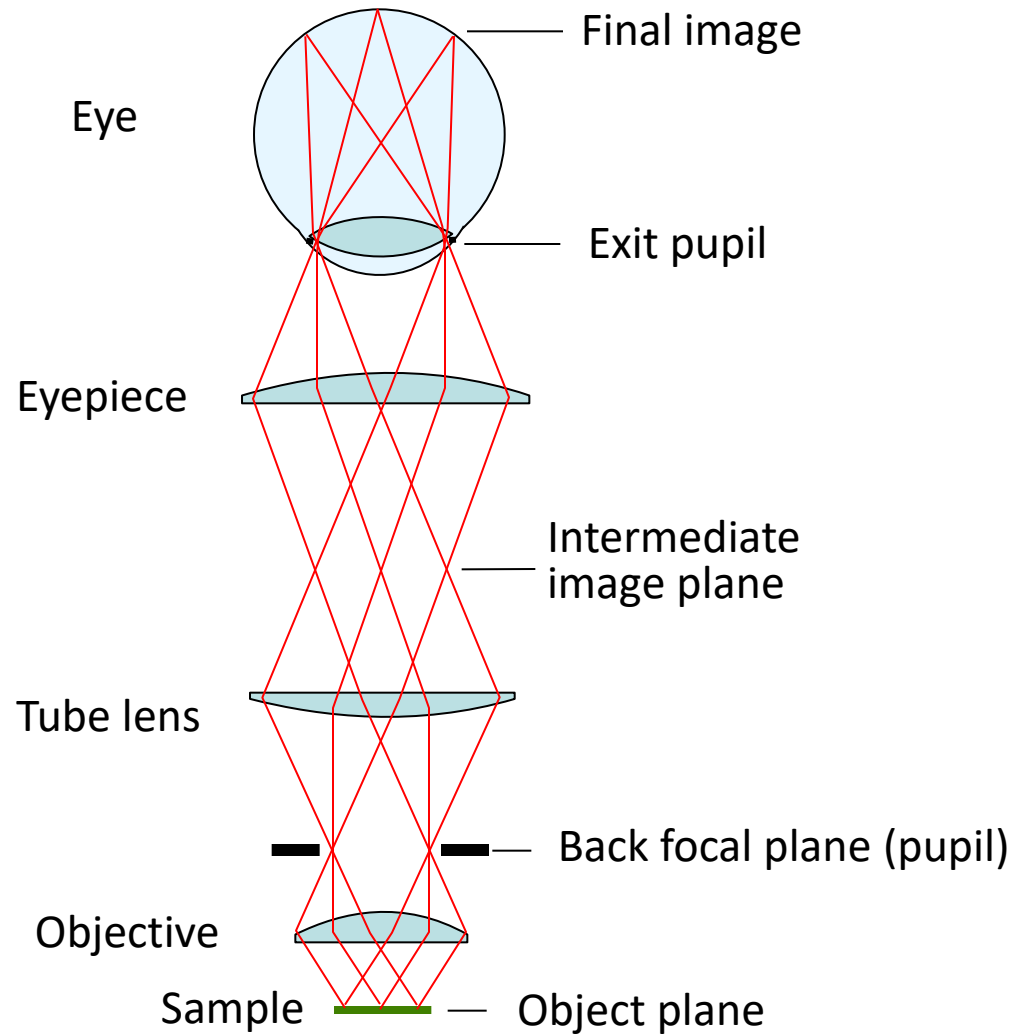


The Compound Microscope

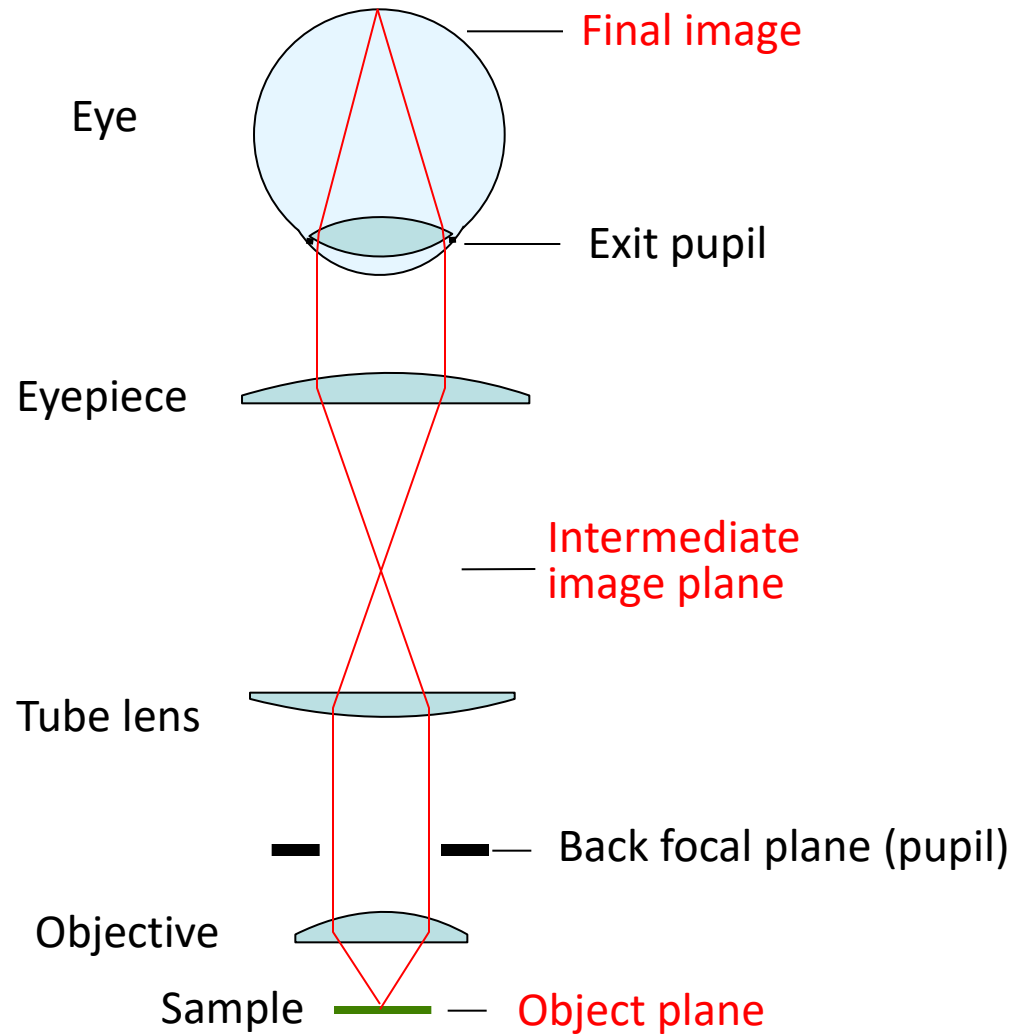


The Compound Microscope

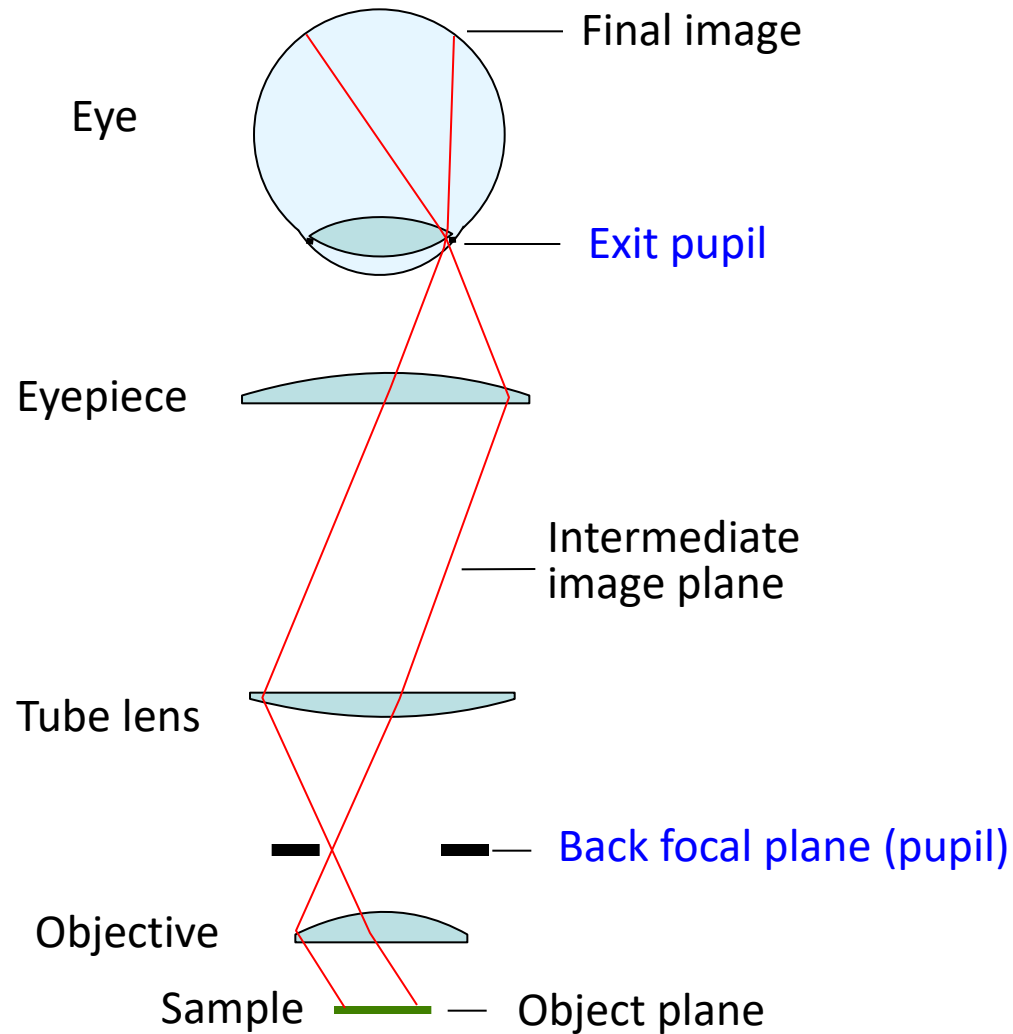

The Compound Microscope

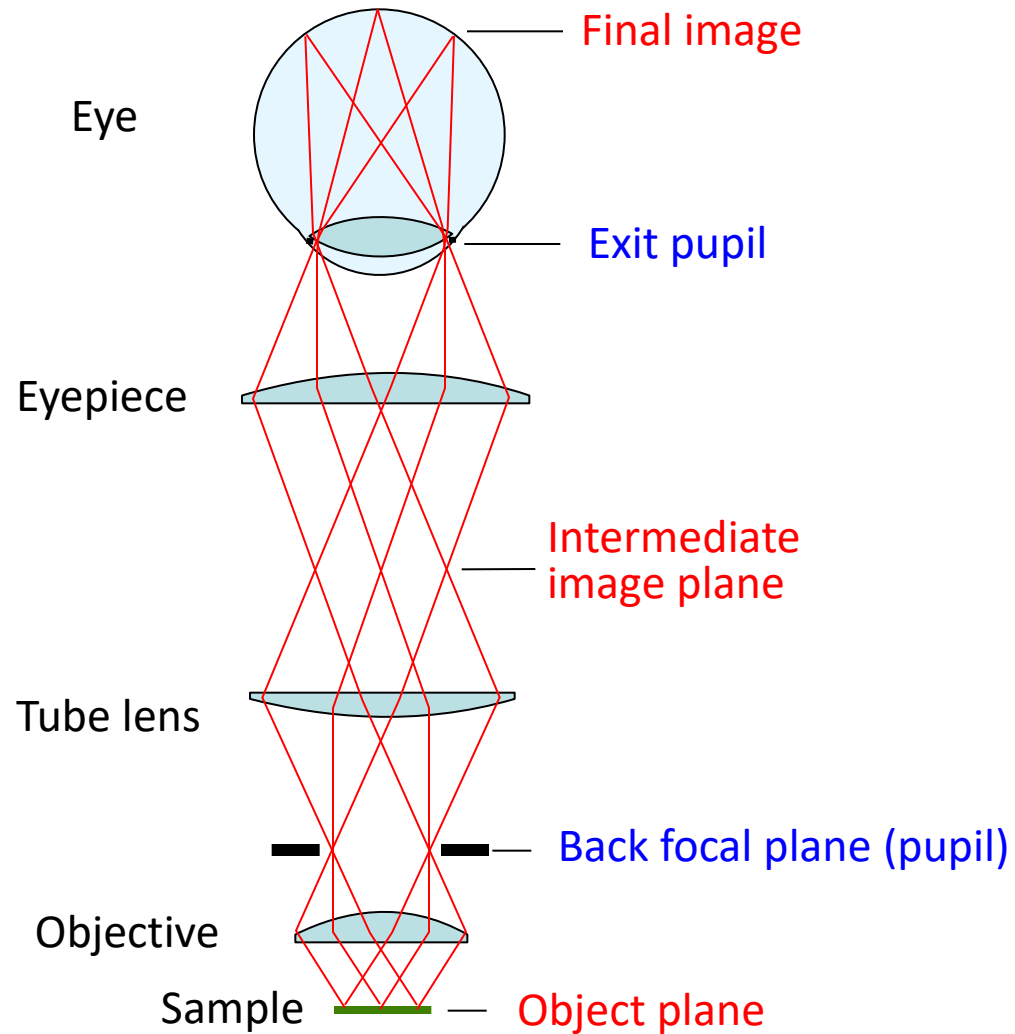

The Compound Microscope

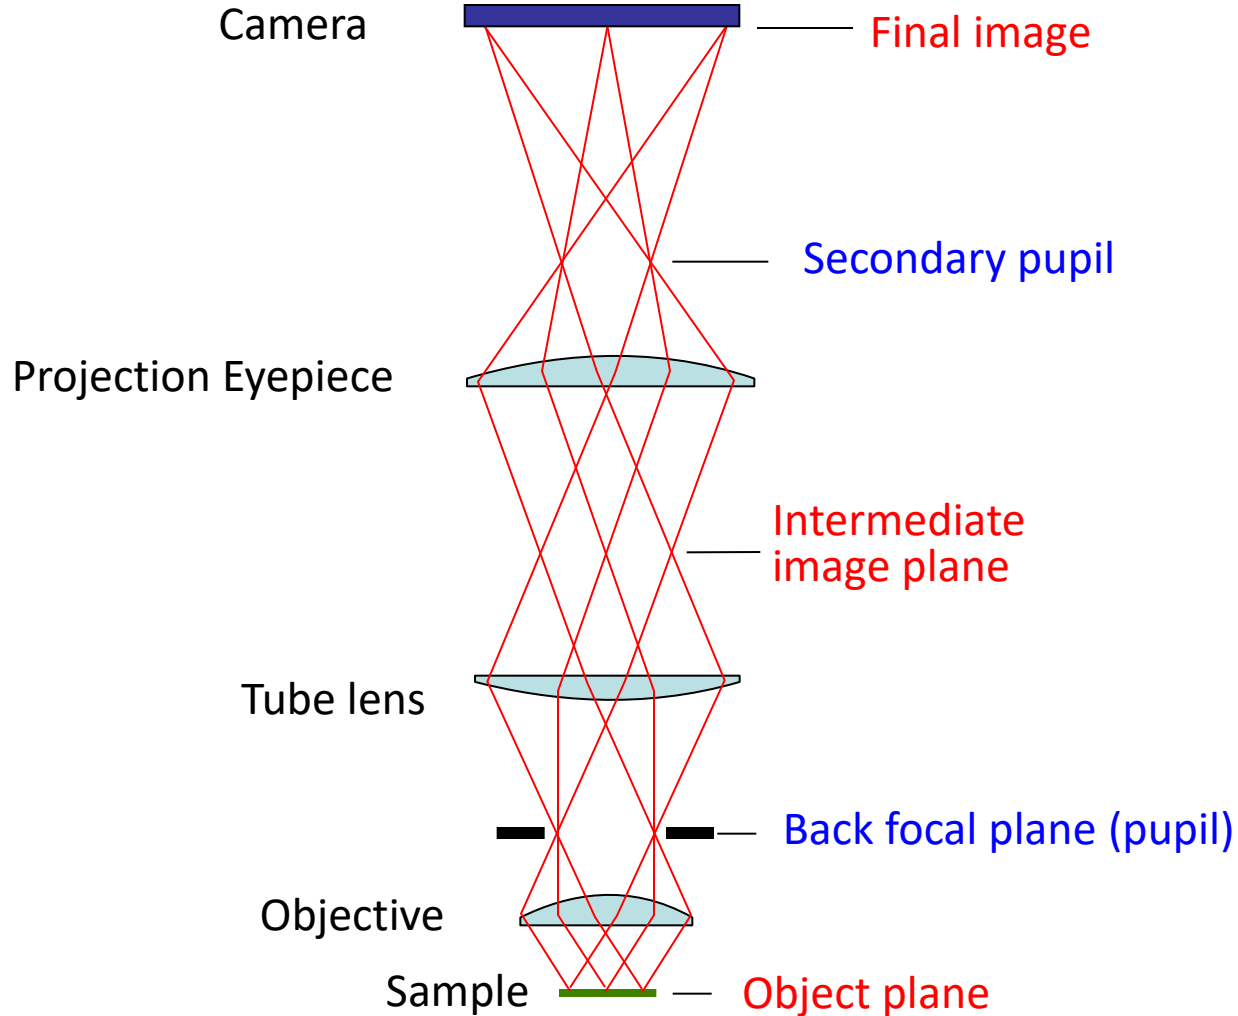

Eyepieces (Oculars)


Aberration-Free 10x Eyepiece With Diopter Adjustment




Features

- Magnification (10x typical)
- “High eye point” (exit pupil high enough to allow eyeglasses)
- Diopter adjust (at least *one* must have this)
- Reticle or fitting for one
- Eye cups

Trans-illumination Microscope

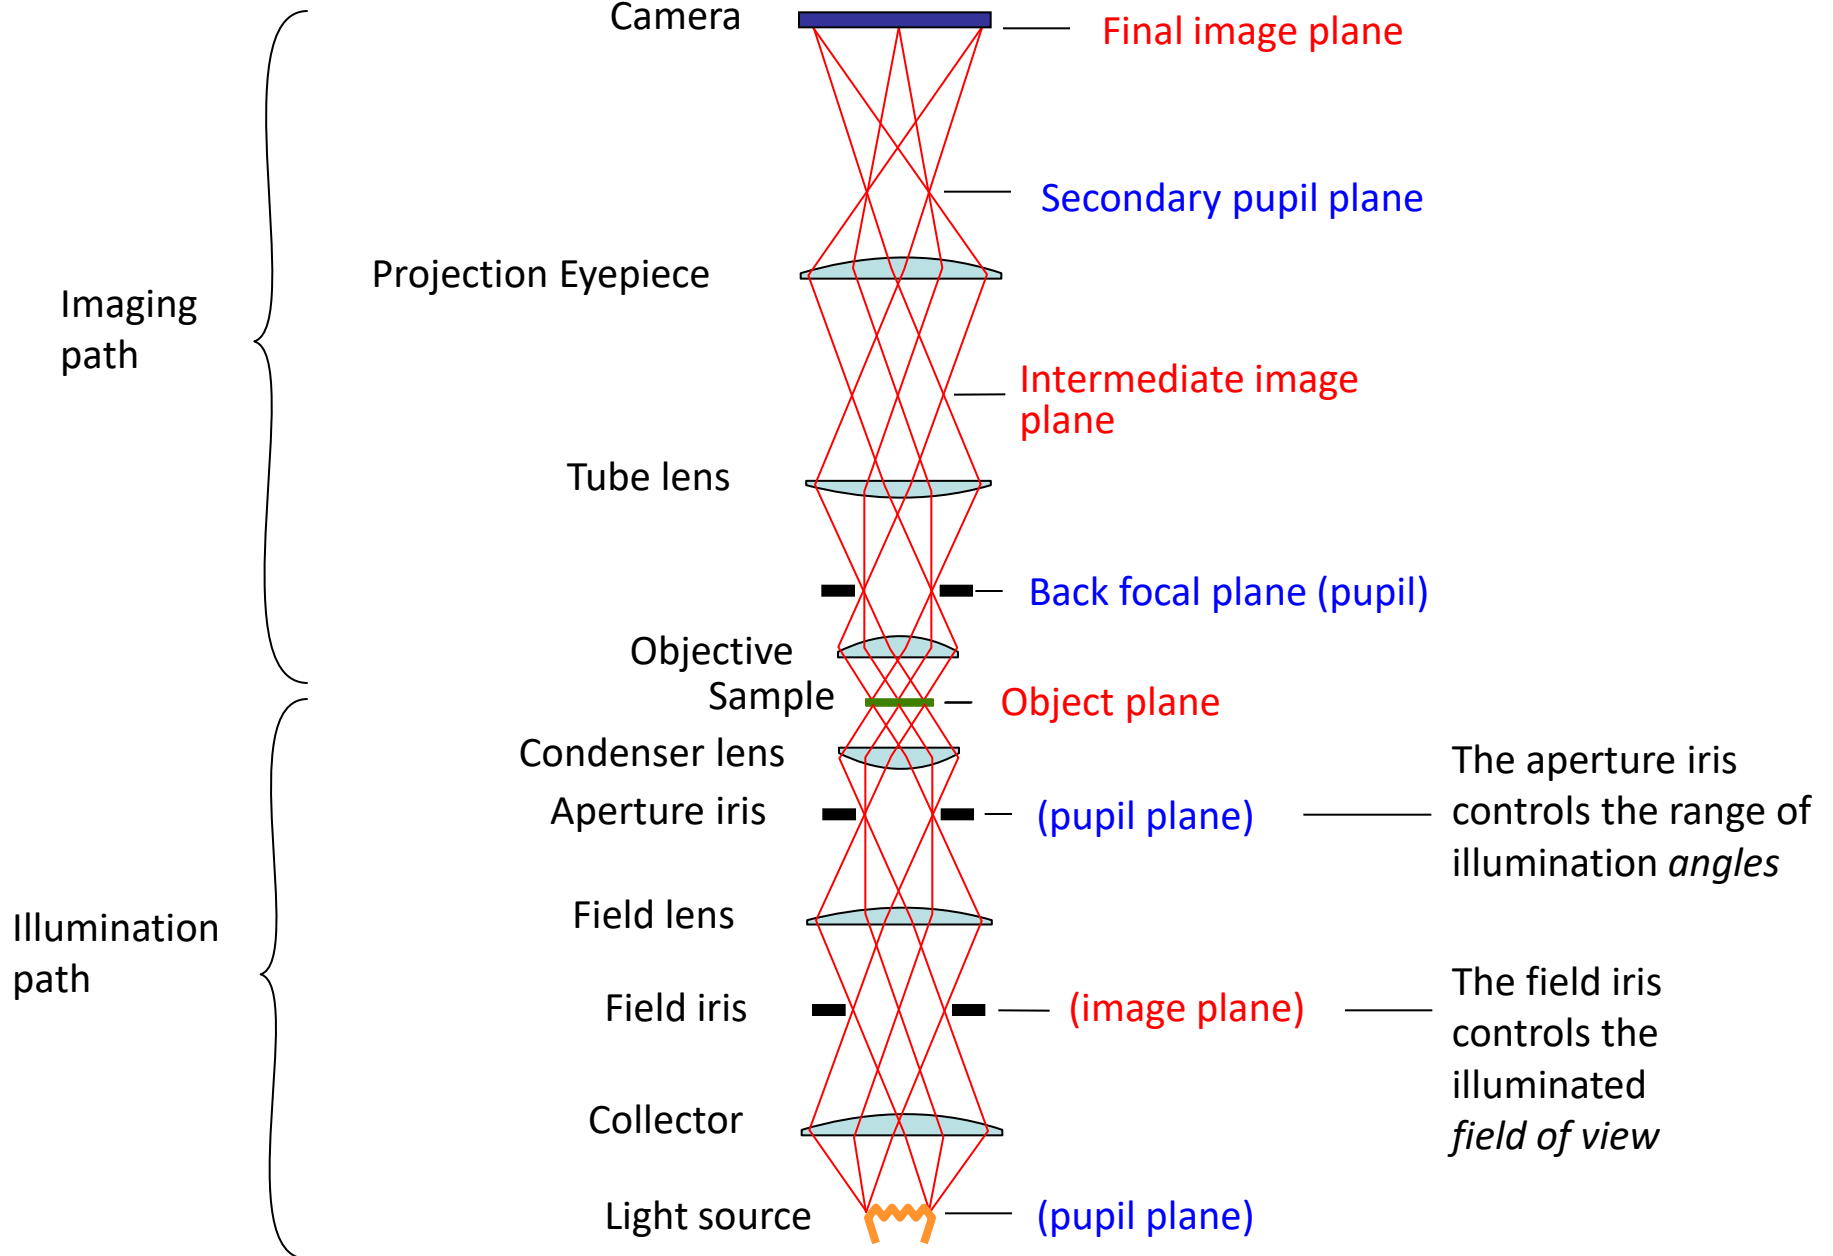


Köhler Illumination

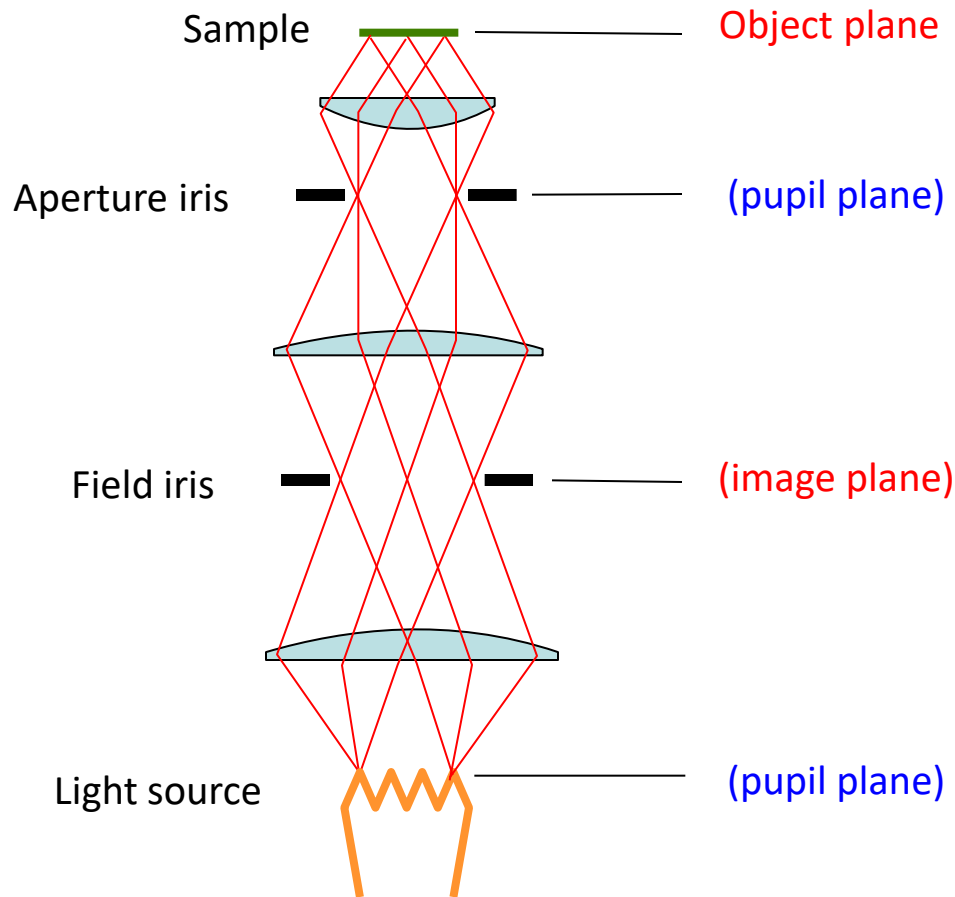

- Each light source point produces a parallel beam of light at the sample
- Uniform light intensity at the sample even if the light source is “ugly” (e.g. a filament)

Critical Illumination

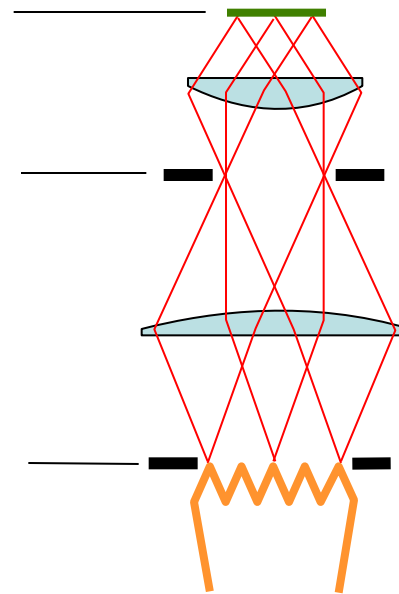

- The source is imaged onto the sample
- Usable only if the light source is perfectly uniform

Conjugate Planes in A Research Microscope

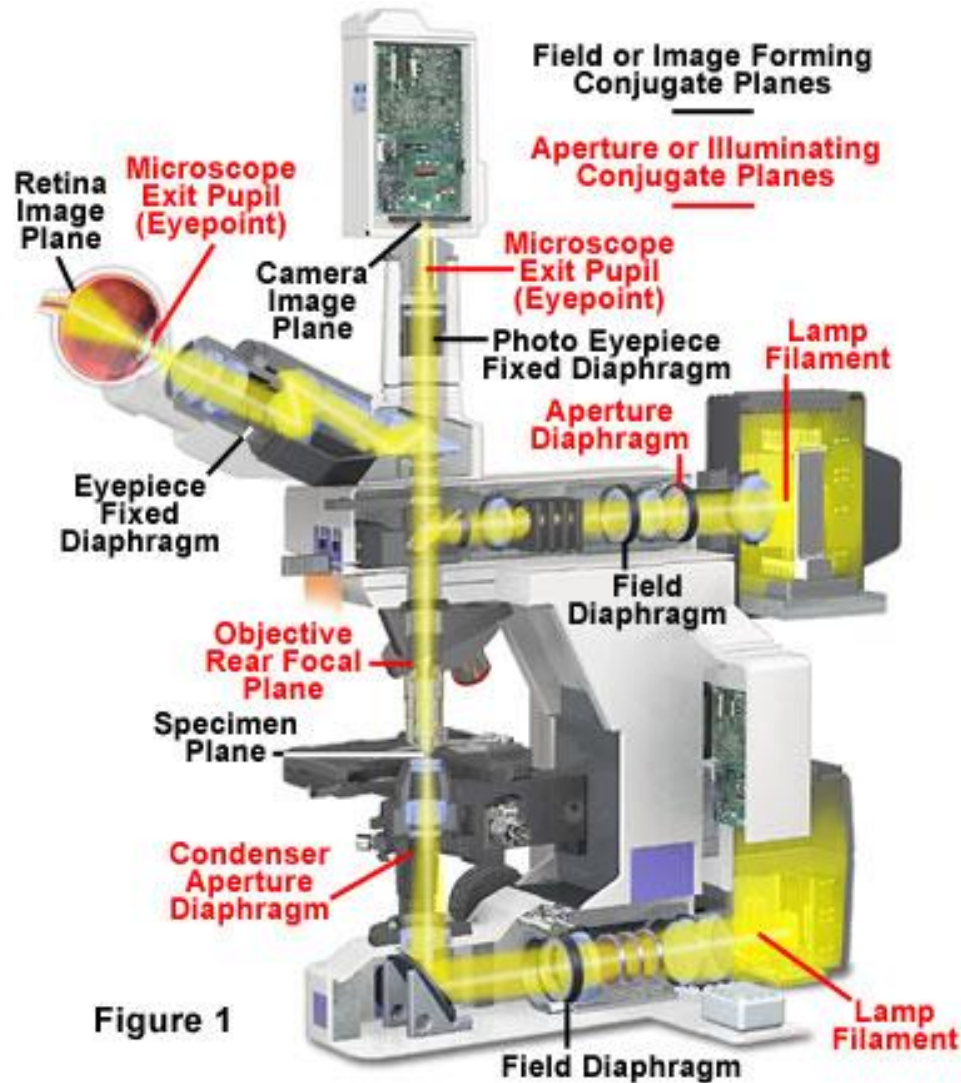


Figure 1

How view the pupil planes?

Two ways:

- “Eyepiece telescope”
- “Bertrand lens”

By far the most important part:
the Objective Lens



Each major manufacturer sells 20-30 different **categories** of objectives.
What are the important distinctions?

Working Distance

Objective Working and Parfocal Distance



In general, high NA lenses have short working distances

However, extra-long working distance objectives do exist


Some examples:

10x/0.3 WD = 15.2mm

20x/0.75 WD = 1.0mm


100x/1.4 WD = 0.13mm

The focal length of a lens depends on the refractive index...

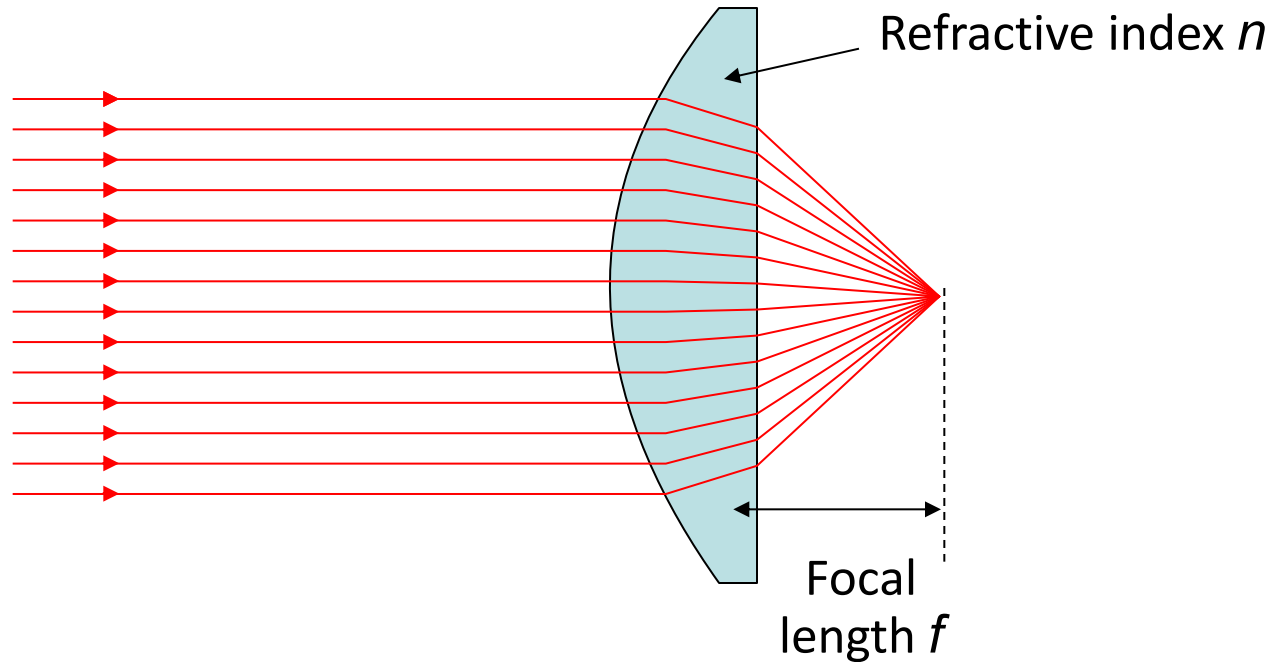


$$f \propto 1/(n-1)$$

... and the refractive index depends on the wavelength (“dispersion”)

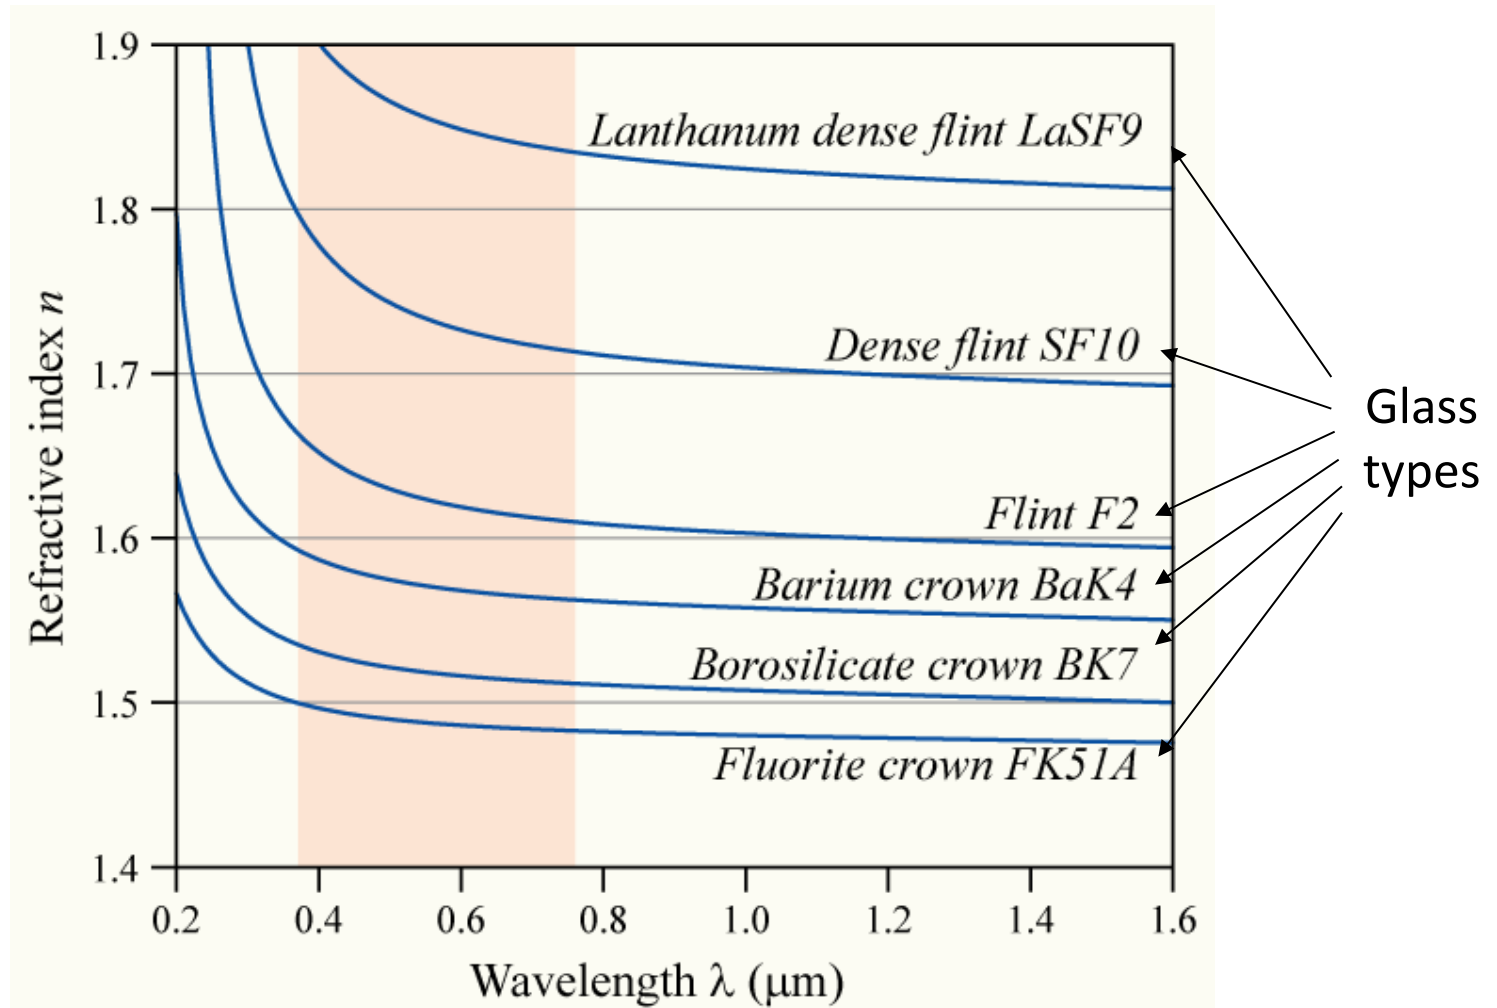


⇒ Chromatic aberration

- Different colors get focused to different planes
- Not good...

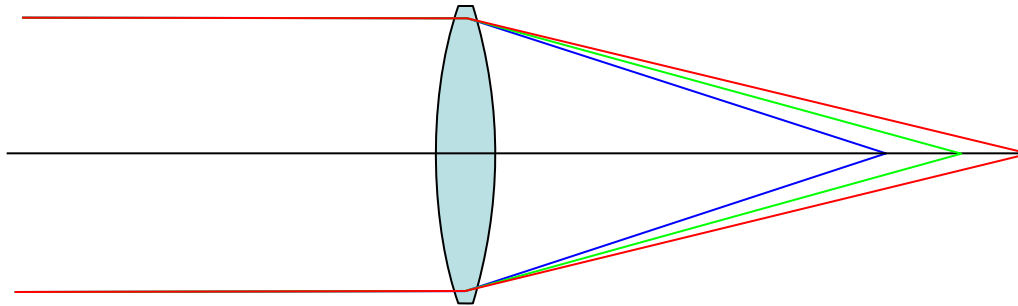


Dispersion vs. refractive index of different glass types

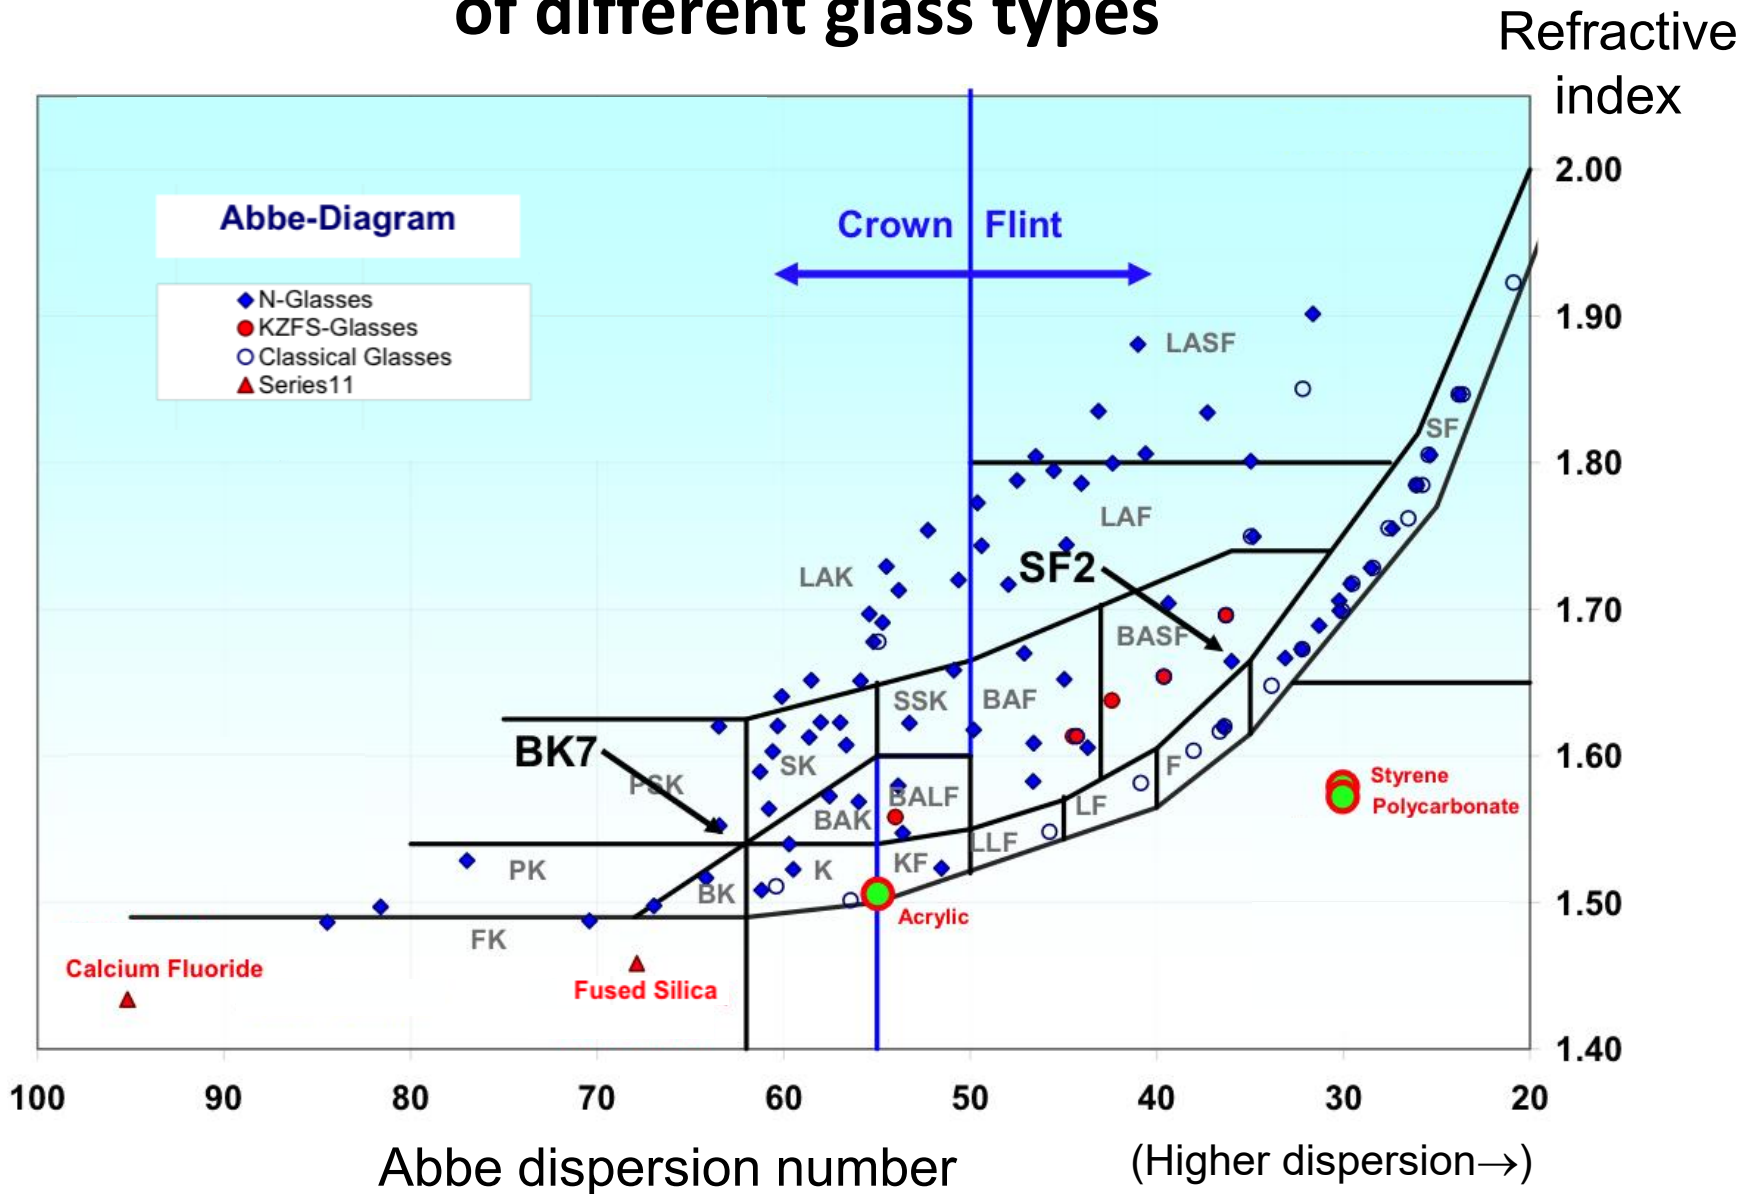


Achromatic Lenses


- Use a weak negative flint glass element to compensate the dispersion of a positive crown glass element

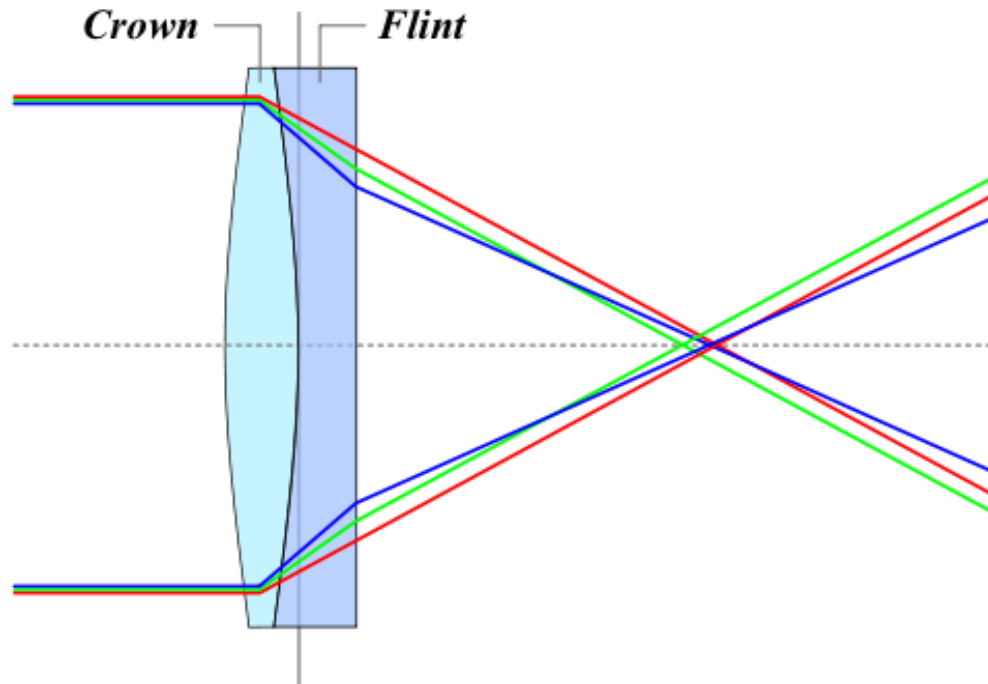

Achromats and Apochromats

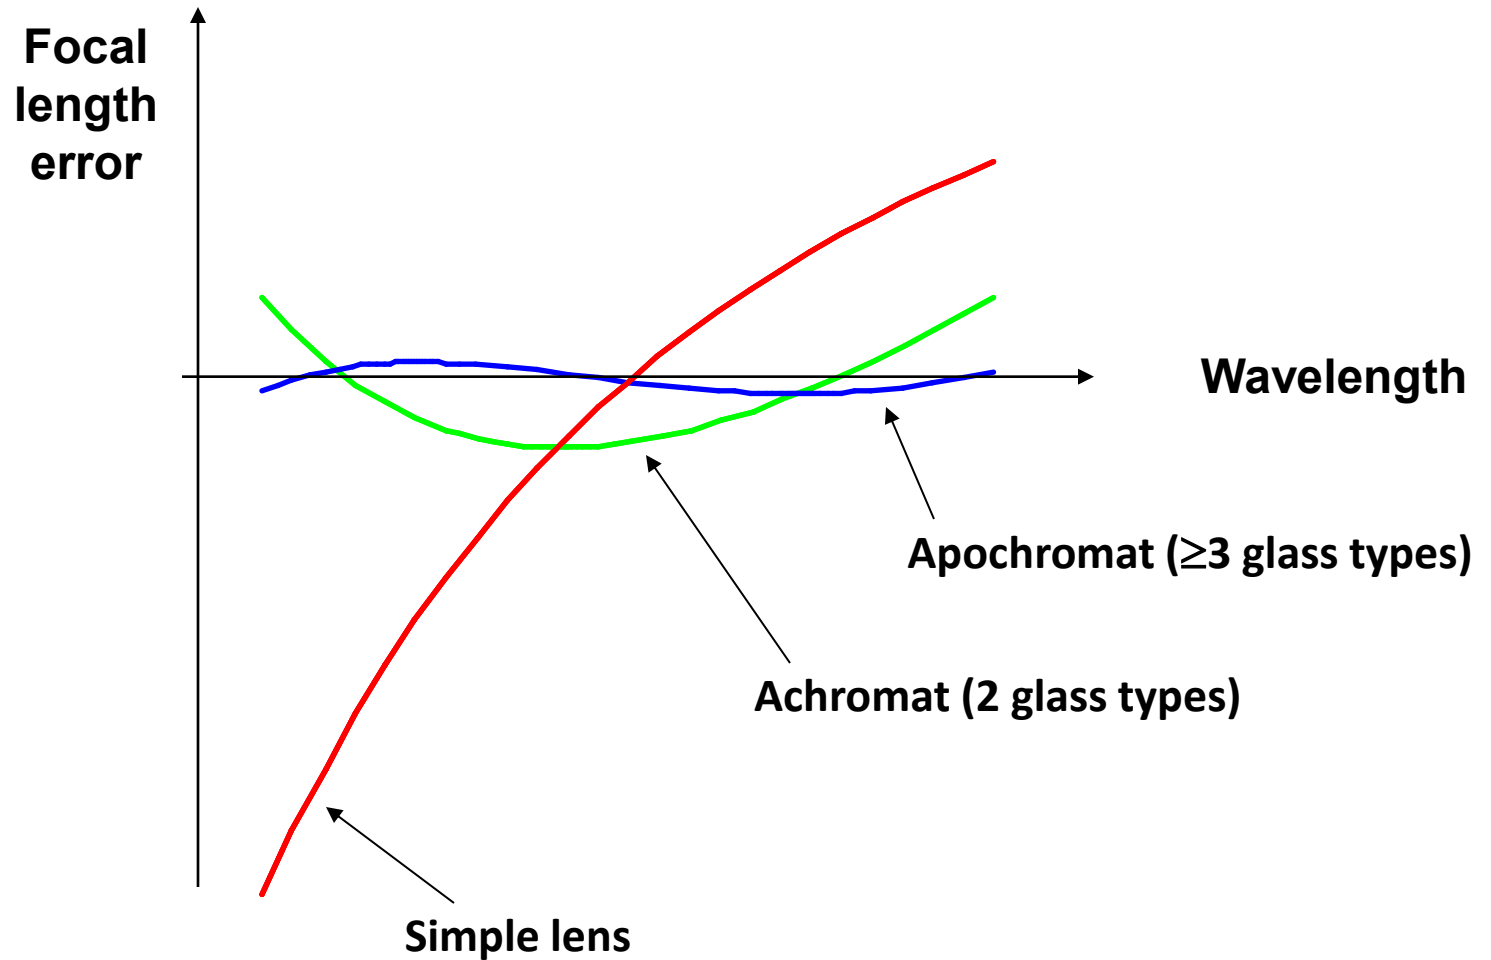


Correction classes of objectives

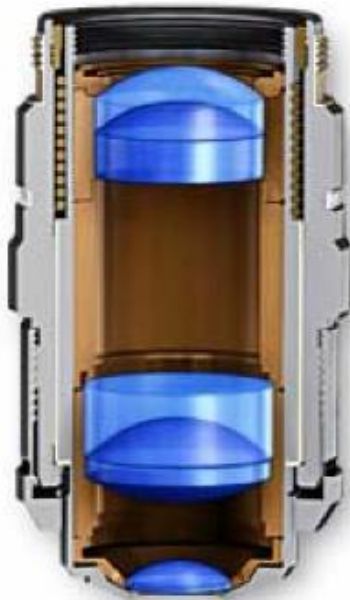

Achromat
(cheap)



Fluor
“semi-apo”
(good correction,
high UV
transmission)


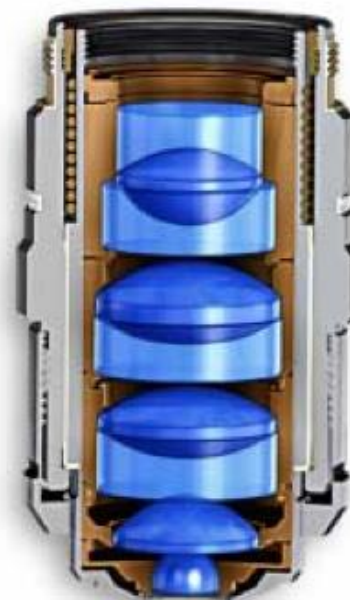


Apochromat
(best correction)

Correction for other (i.e. monochromatic) aberrations
also improves in the same order




Curvature of Field

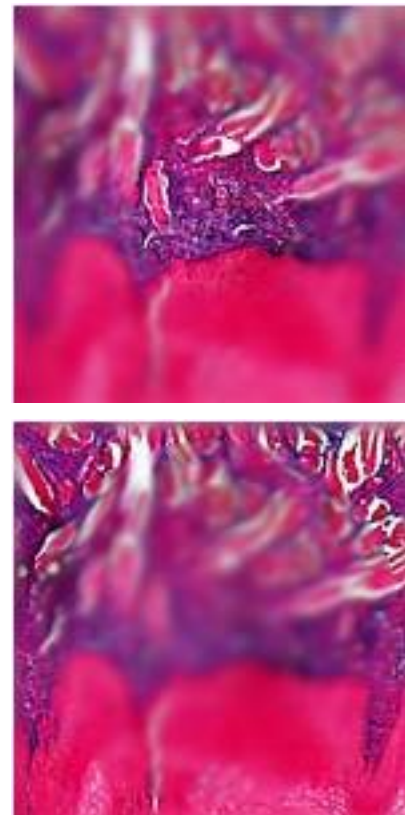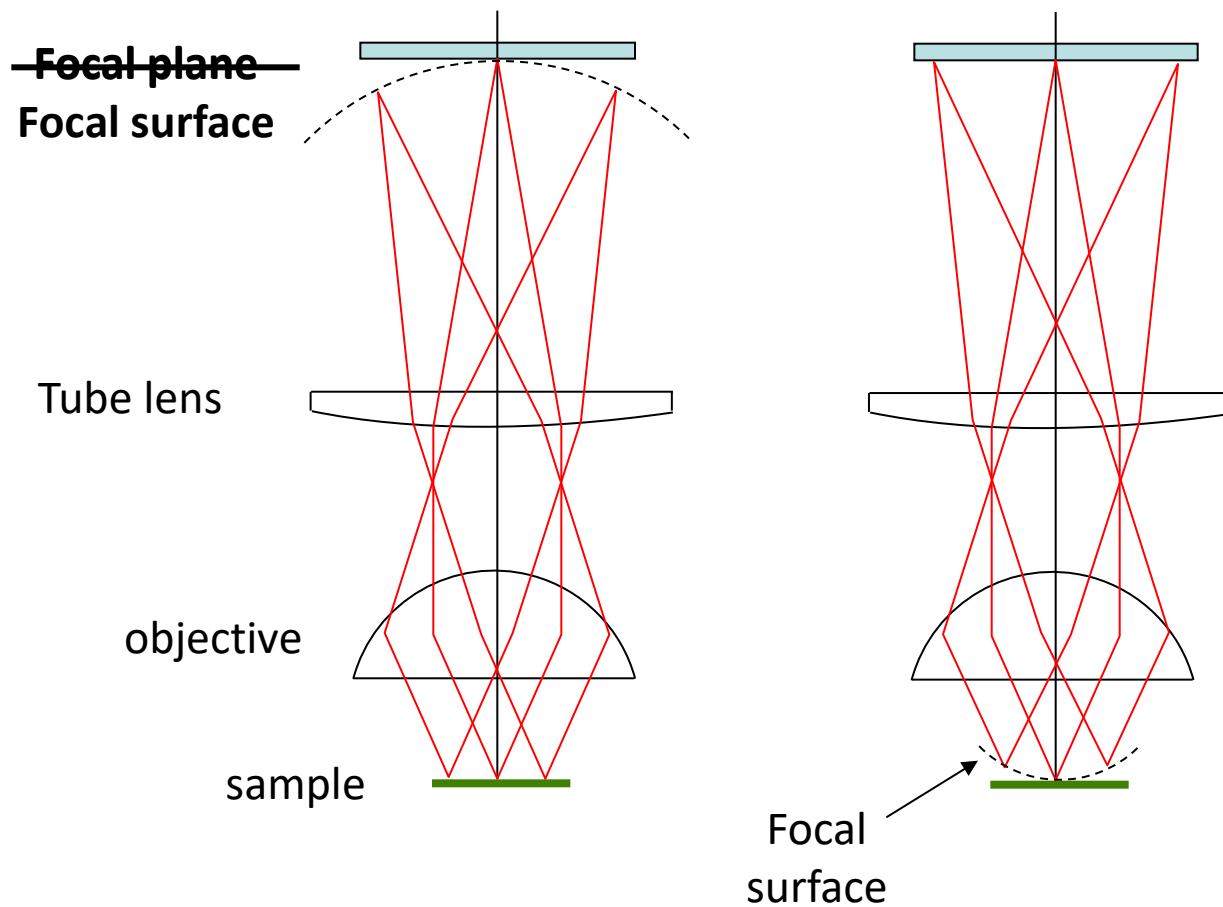

Plan objectives

- Corrected for field curvature
- More complex design
- Needed for most photomicrography

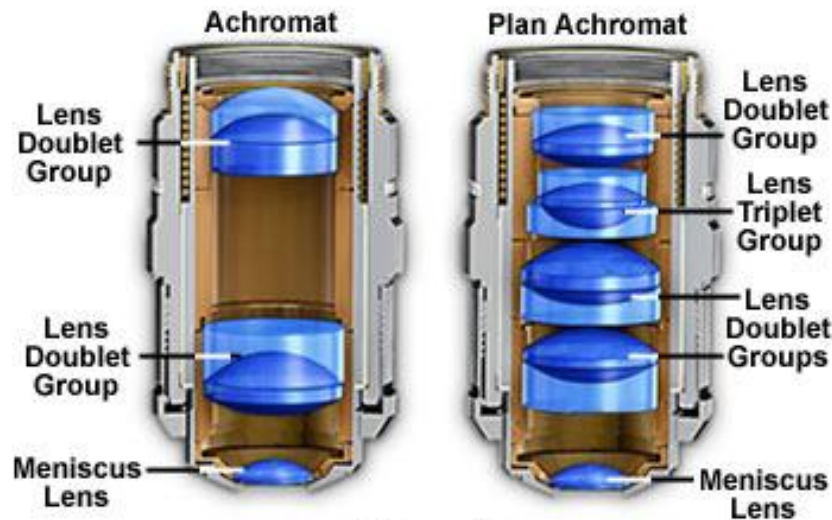


- **Plan-Apochromats** have the highest performance (and highest complexity and price)



What is the Resolution Limit of an Objective?

i.e. what is the smallest separation between two
objects you can detect?

Diffraction by a periodic structure (grating)

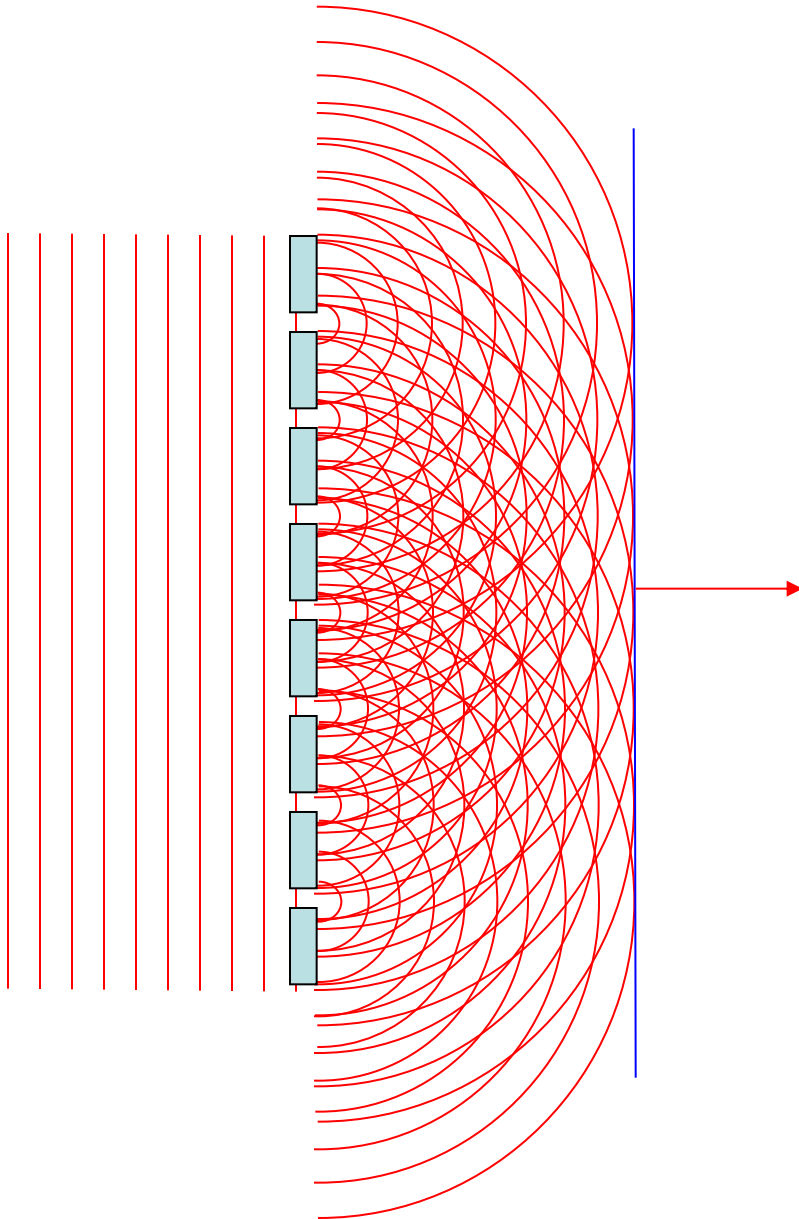

Diffraction by a periodic structure (grating)

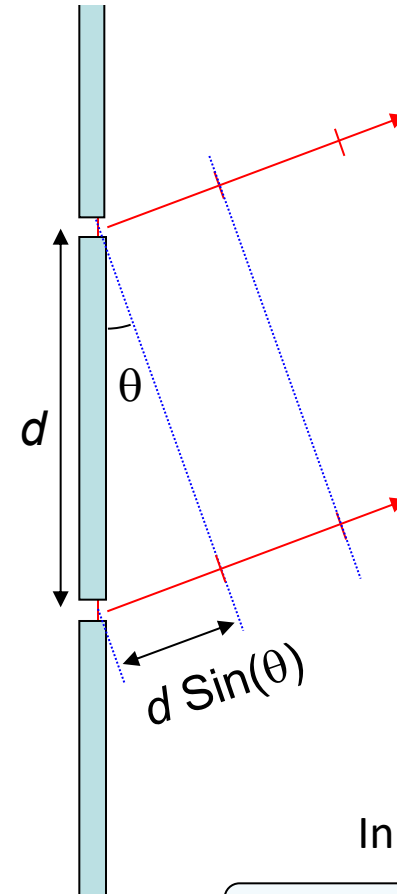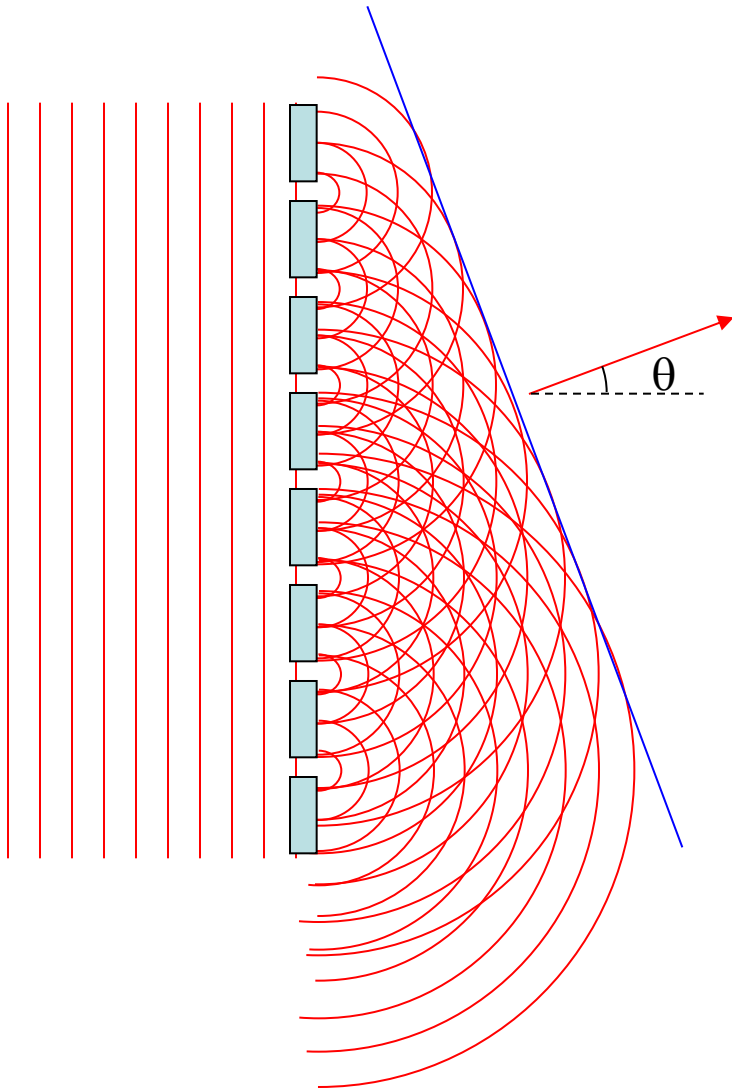

In phase if:

$$d \sin(\theta) = m \lambda$$

for some integer m

Diffraction by an aperture




See “Teaching Waves with Google Earth”


<http://arxiv.org/pdf/1201.0001v1.pdf> for more

Diffraction by an aperture

drawn as waves

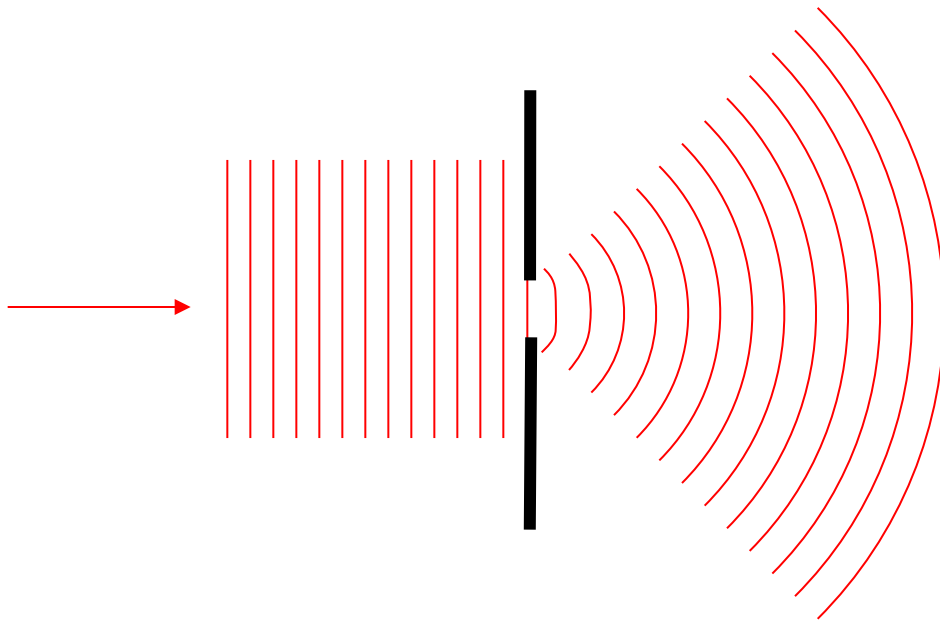

Light spreads to new angles

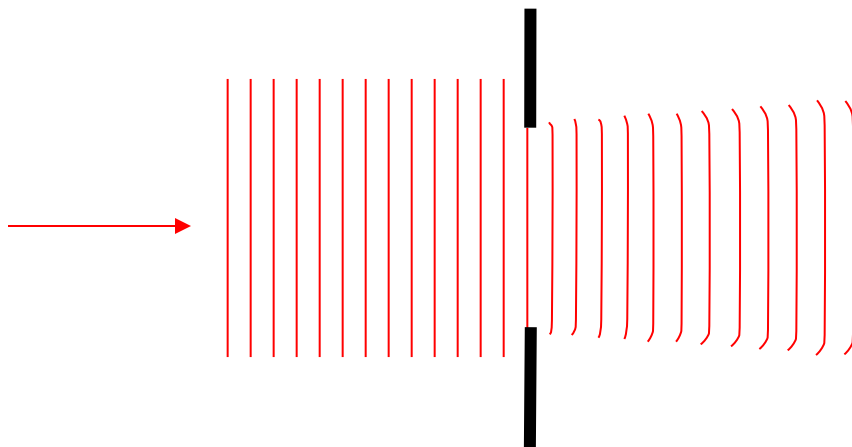


Larger aperture





weaker diffraction

Diffraction by an aperture

drawn as rays

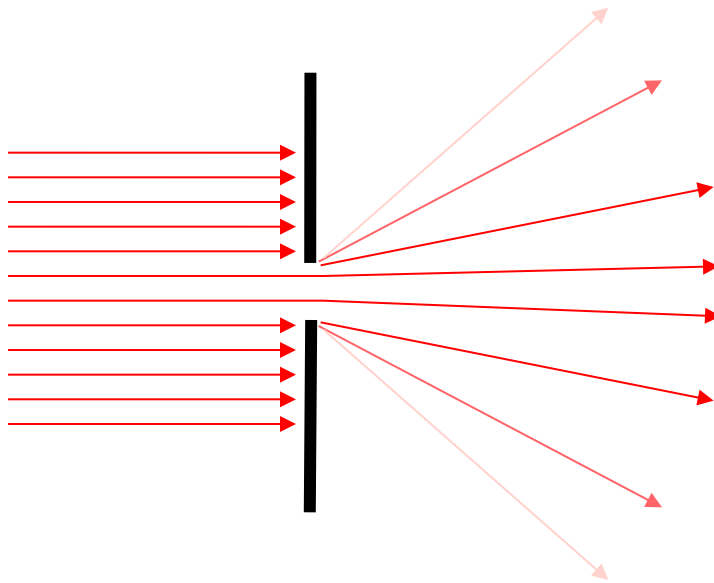

The pure, “far-field”
diffraction pattern
is formed at ∞ distance...

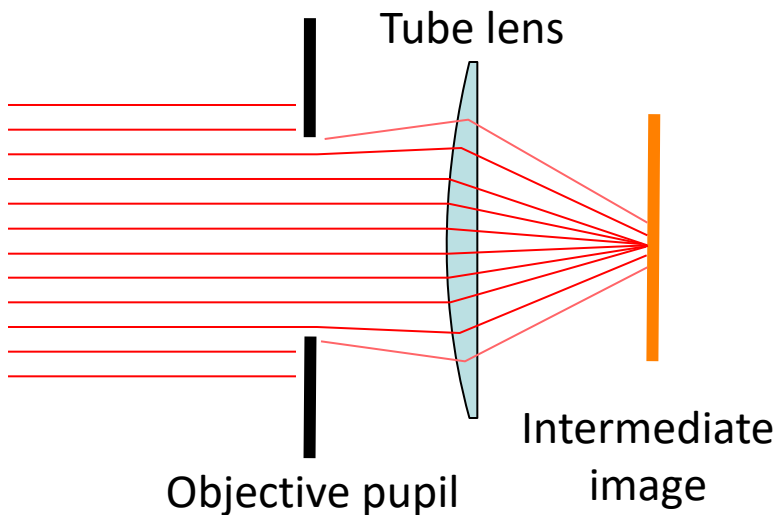
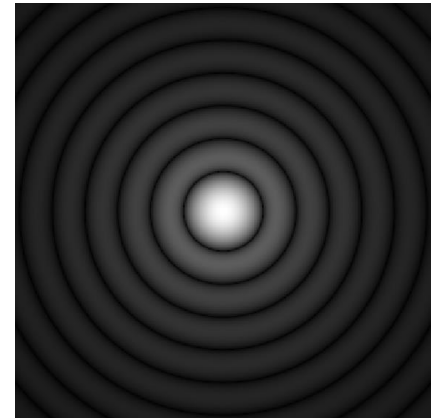


...or can be formed
at a finite distance
by a lens...


...as happens in a microscope

The Airy Pattern


= the far-field diffraction pattern from a round aperture

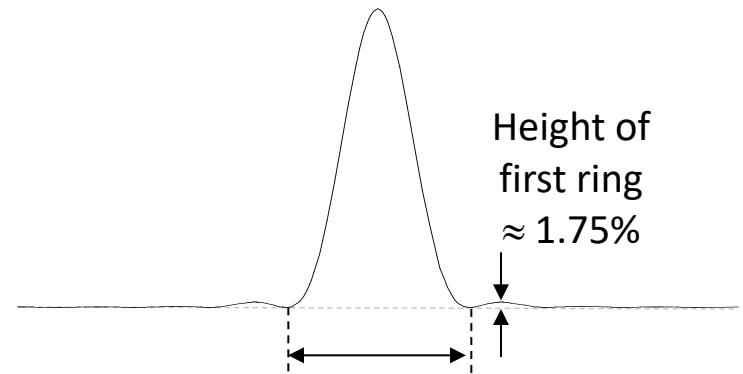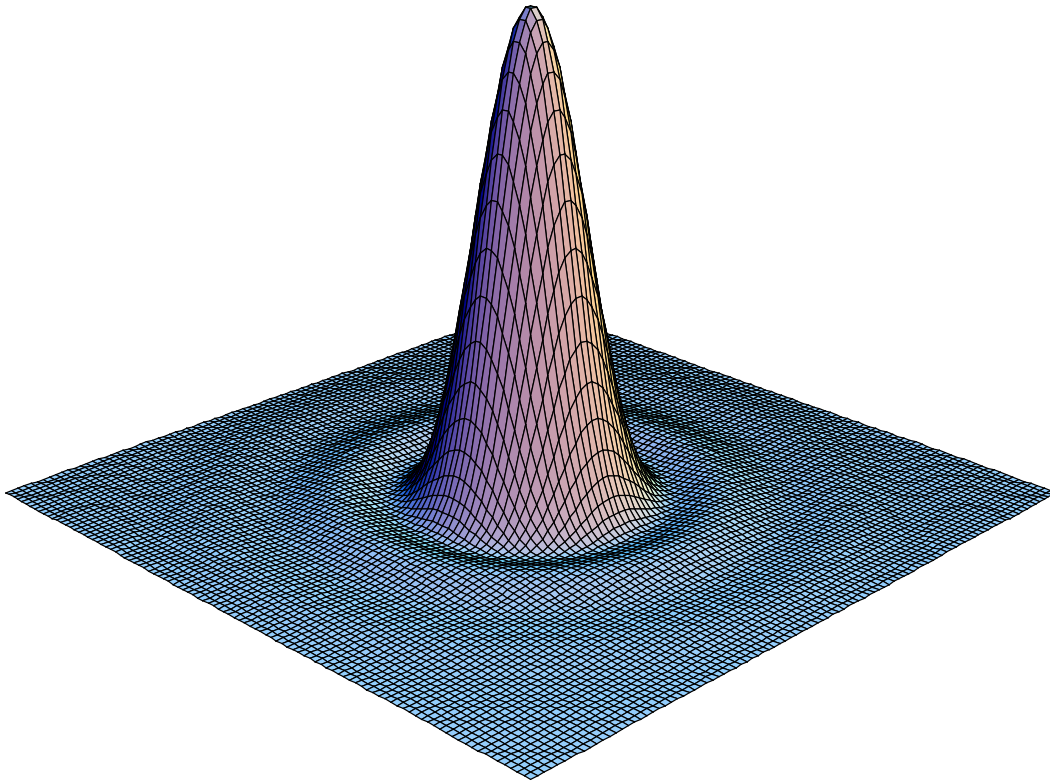


"Airy disk" diameter
 $d = 2.44 \lambda f/d$
(for small angles d/f)

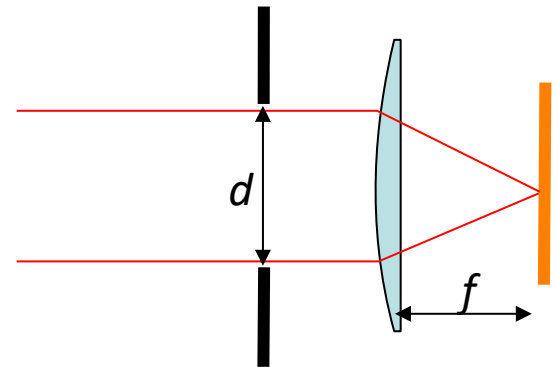


Aperture and Resolution

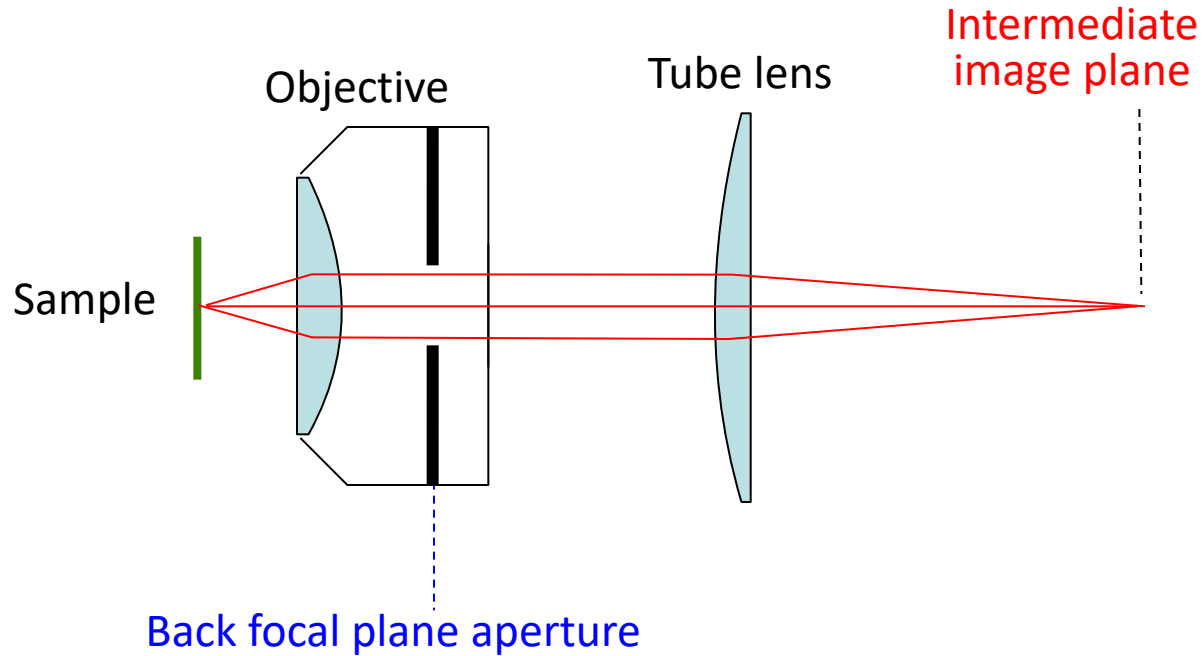


Diffraction spot
on image plane
= *Point Spread Function*

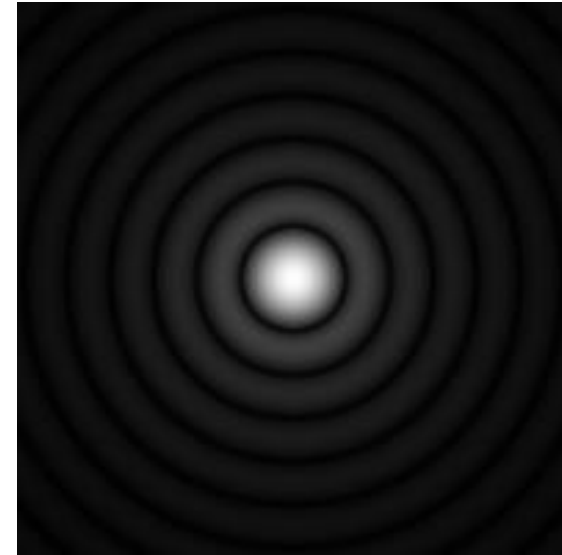


Aperture and Resolution

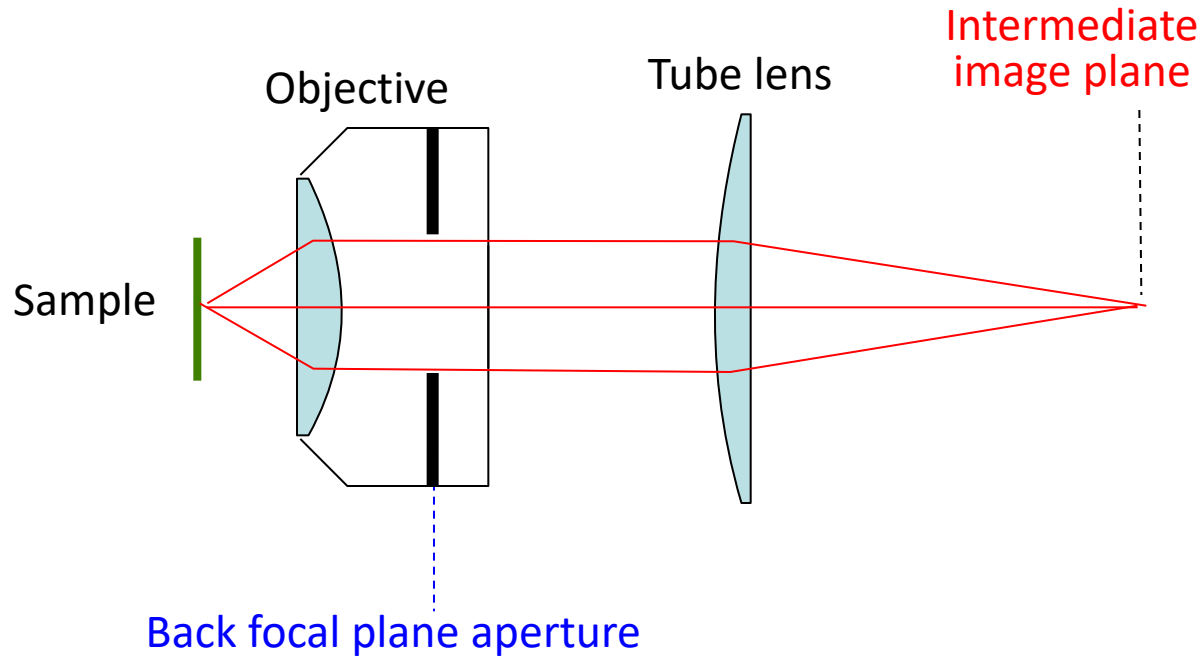


Diffraction spot
on image plane
= *Point Spread Function*

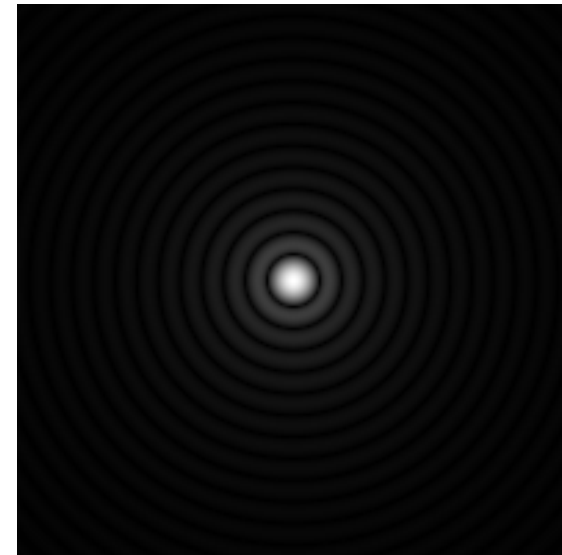


Aperture and Resolution

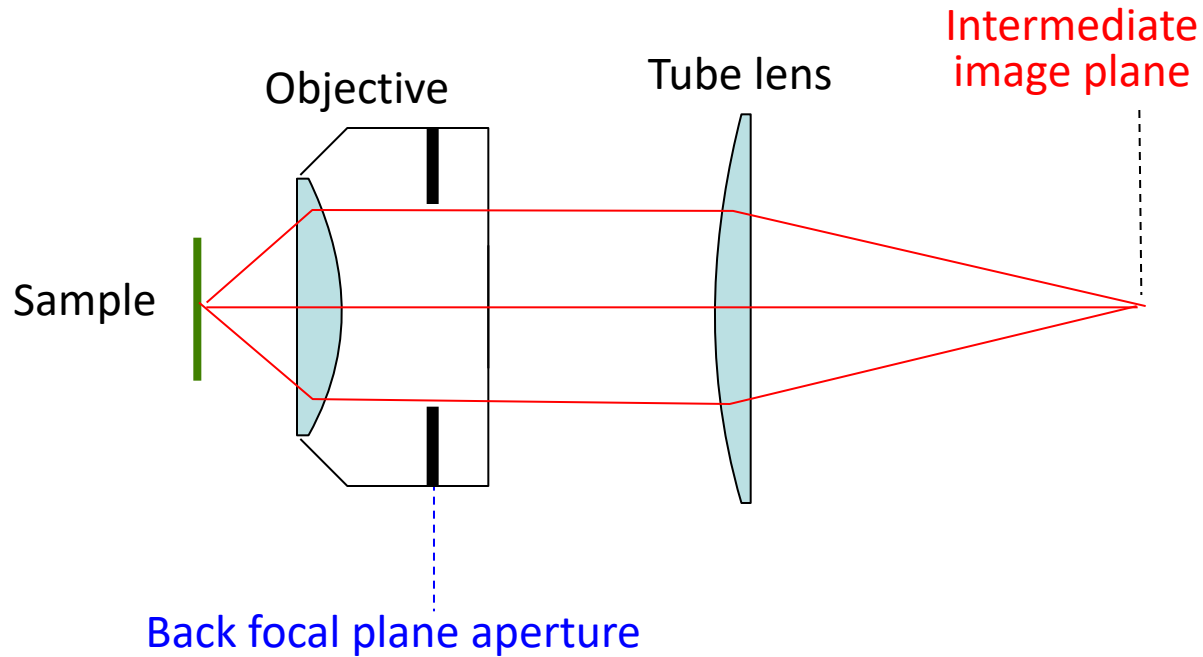


Diffraction spot
on image plane
= *Point Spread Function*

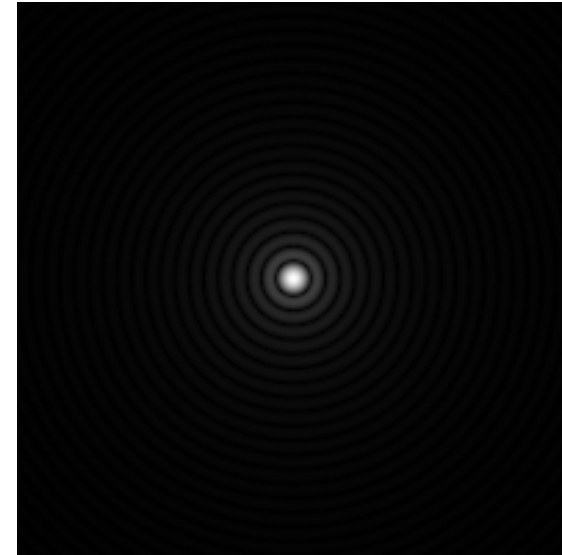

Aperture and Resolution

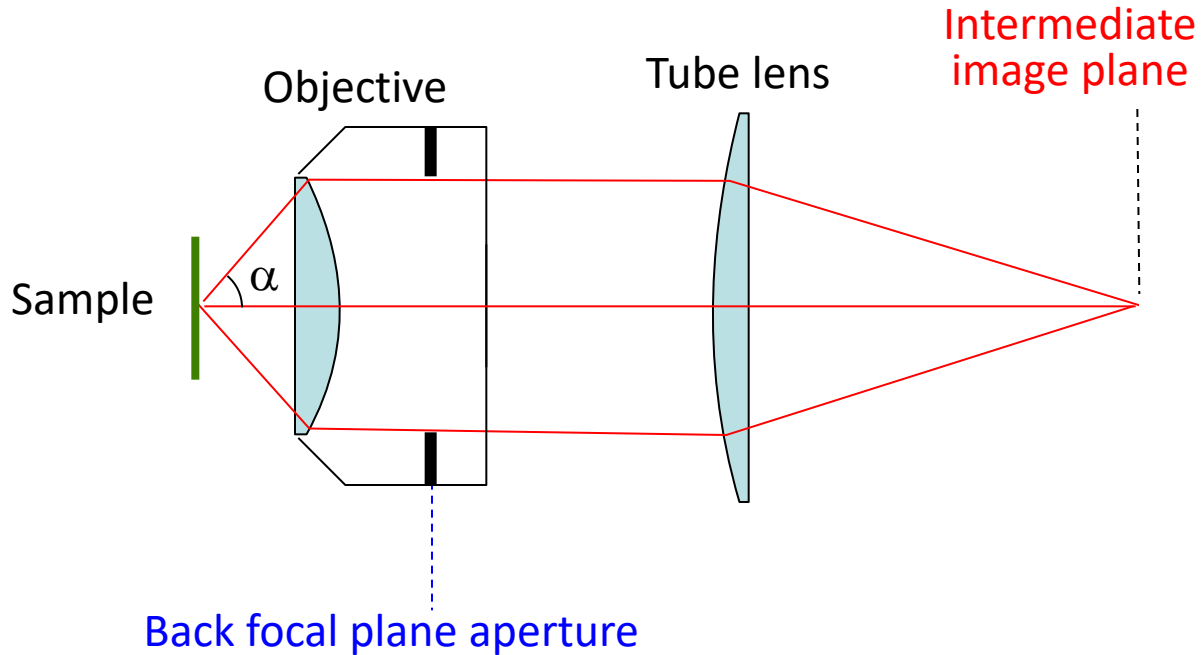

Diffraction spot
on image plane
(resolution)

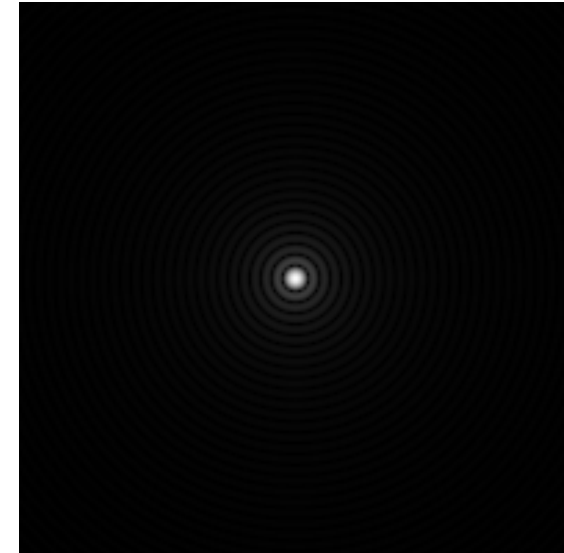

- Image resolution improves with aperture size — Numerical Aperture (NA)


$$NA = n \sin(\alpha)$$

where:


α = light gathering angle

n = refractive index of sample

Numerical Aperture

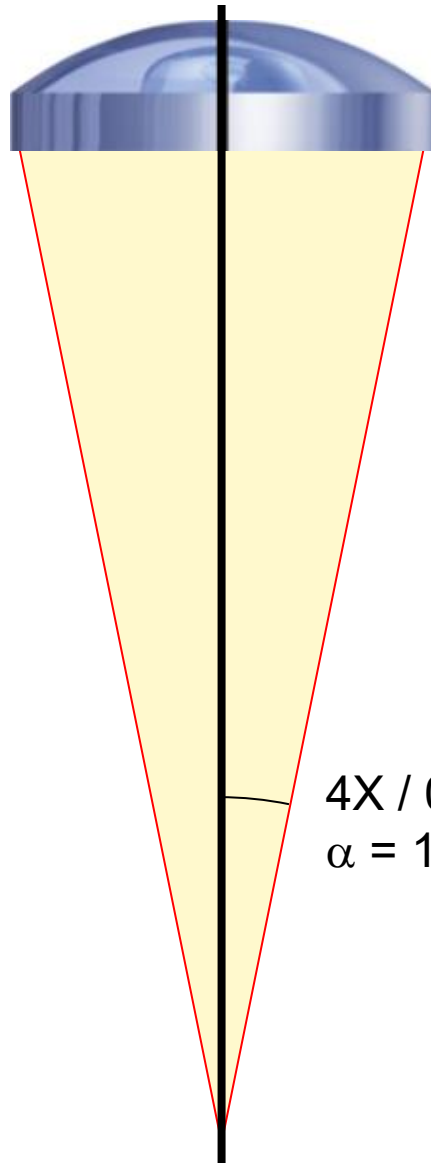


4X / 0.20 NA
 $\alpha = 11.5^\circ$



100X / 0.95 NA
 $\alpha = 71.8^\circ$

Immersion Objectives

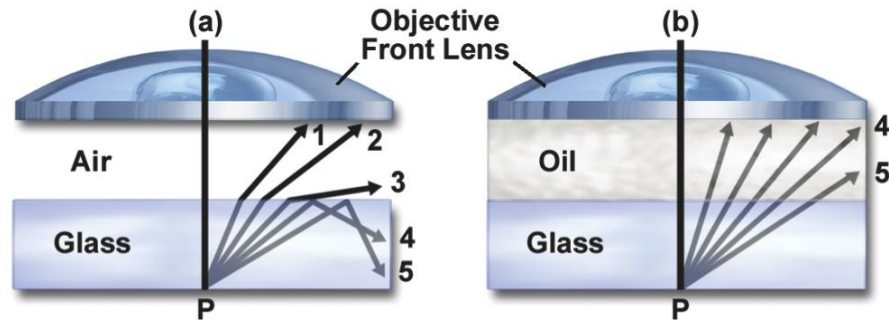

⇒ NA cannot exceed
the *lowest* n between the
sample and the objective lens

⇒ $NA > 1$ requires **fluid immersion**

NA can approach
the index of the
immersion fluid

Oil immersion:

$n \approx 1.515$

max NA ≈ 1.4 (1.45–1.49 for TIRF)

Glycerol immersion:

$n \approx 1.45$ (85%)

max NA ≈ 1.35 (Leica)

Water immersion:


$n \approx 1.33$

max NA ≈ 1.2

Resolution

Ernst Abbe's argument (1873)

Consider a striped sample $\approx$ a diffraction grating

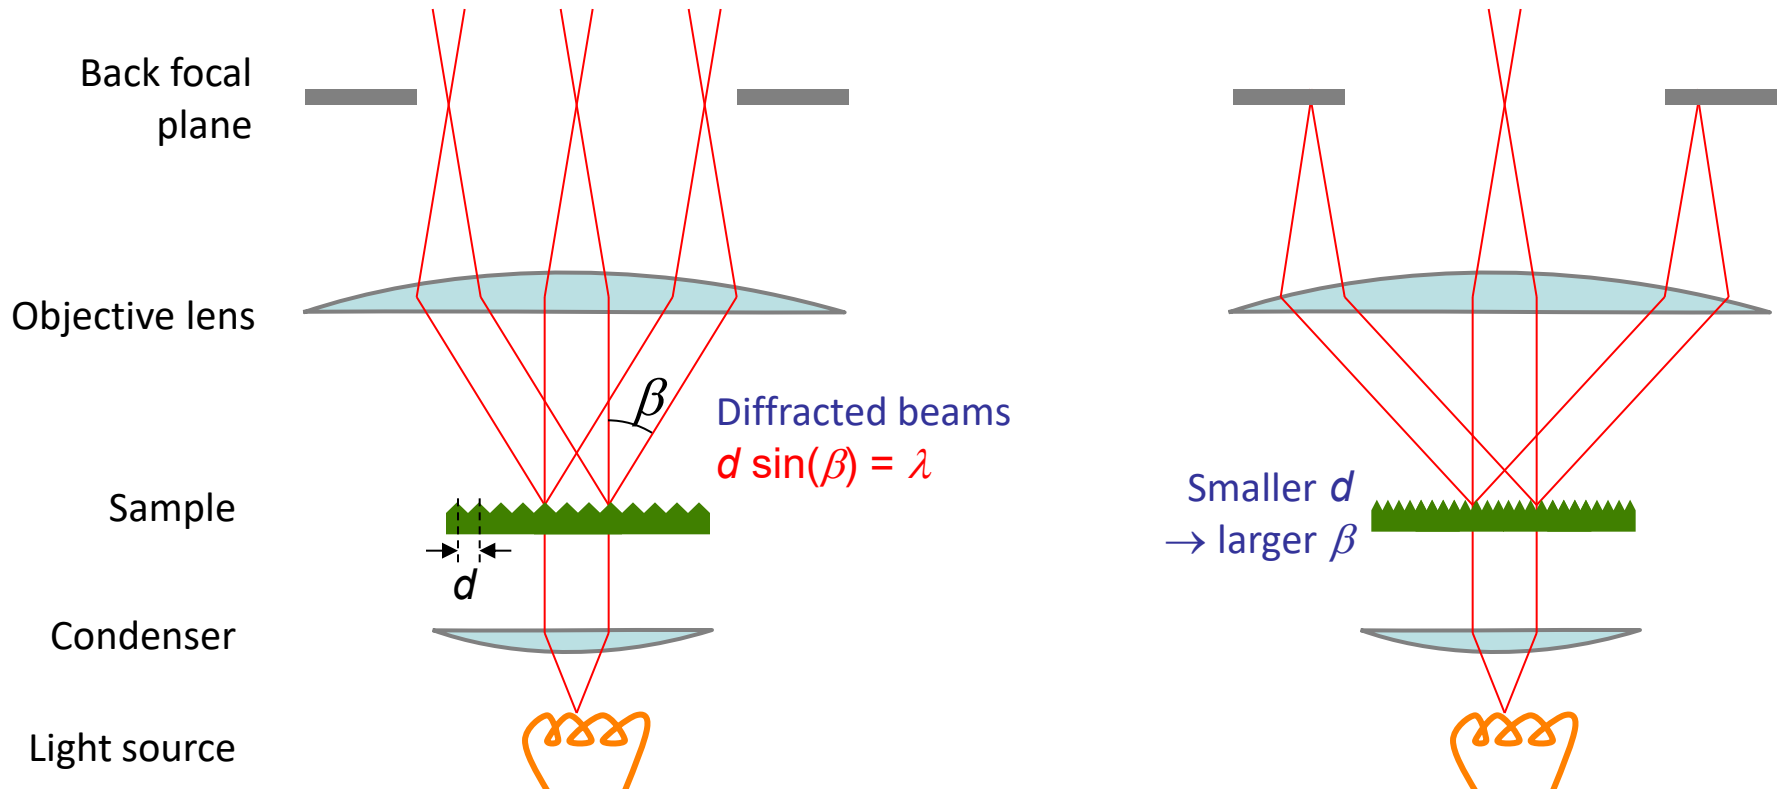


If $\beta > \alpha$, only one spot makes it through
 $\Rightarrow$ no interference $\Rightarrow$ no image formed

Resolution (smallest resolvable d):

$$d_{\min} = \lambda_{\text{sample}} / \sin(\alpha) = \lambda / n \sin(\alpha) = \lambda / NA$$

(Abbe's argument, continued)

Now consider oblique illumination
(an off-axis source point):

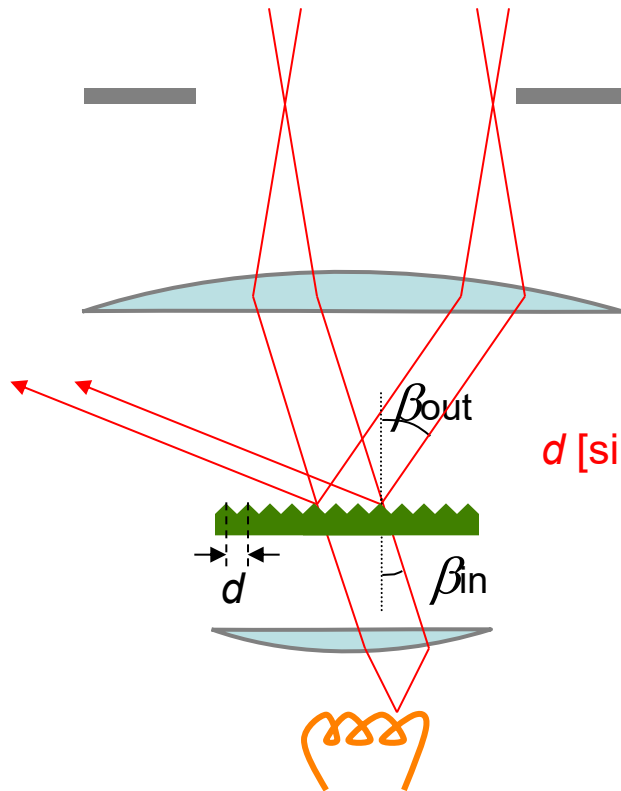

One spot hopelessly lost,
but **two** spots get through
→ interference → image formed!

$$d [\sin(\beta_{in}) + \sin(\beta_{out})] = \lambda$$

Two spots get through if
 $\beta_{out} < \alpha$ and $\beta_{in} < \alpha$.


Resolution (smallest resolvable d)
with incoherent illumination (all possible illumination directions):

$$d_{min} = \lambda / (NA_{obj} + NA_{condenser})$$

→ $\lambda/2 NA$ if $NA_{condenser} \geq NA_{obj}$ ("Filling the back focal plane")

Aperture, Resolution & Contrast

Can adjust the condenser NA with the **aperture iris**

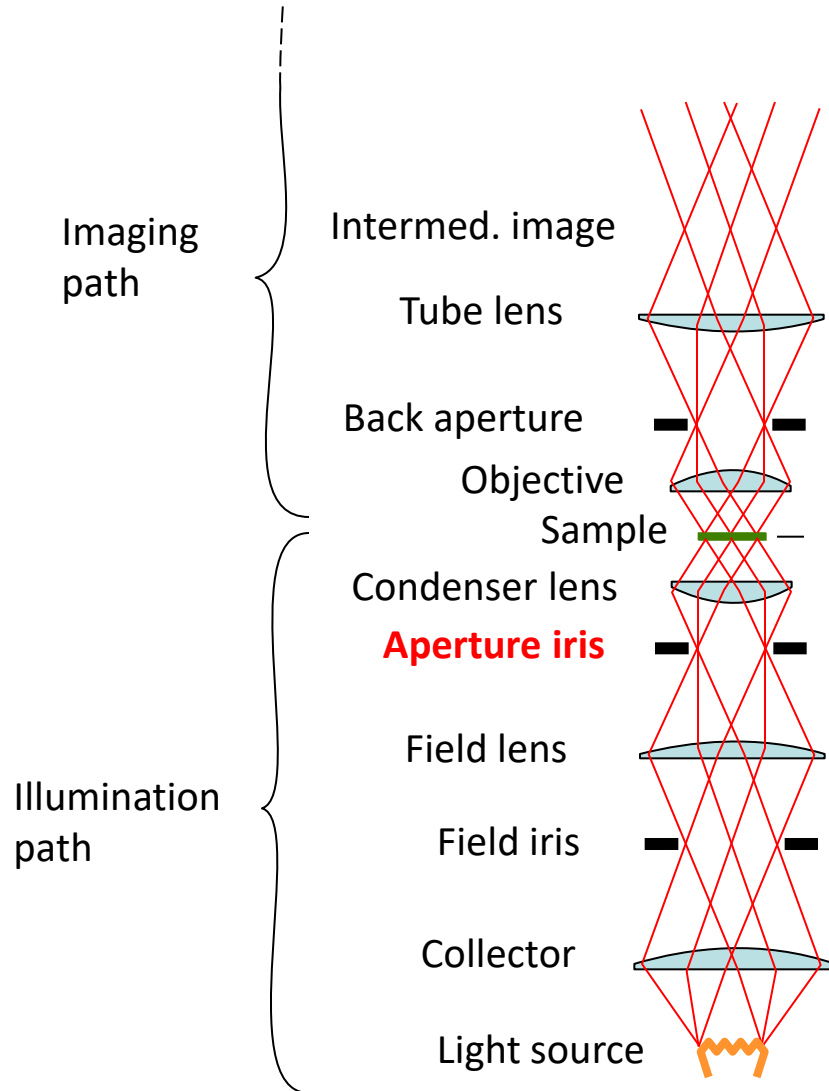


Q: Don't we always want it full open??


A: **No**

Why? Tradeoff:
resolution vs. **contrast**

NA and Resolution

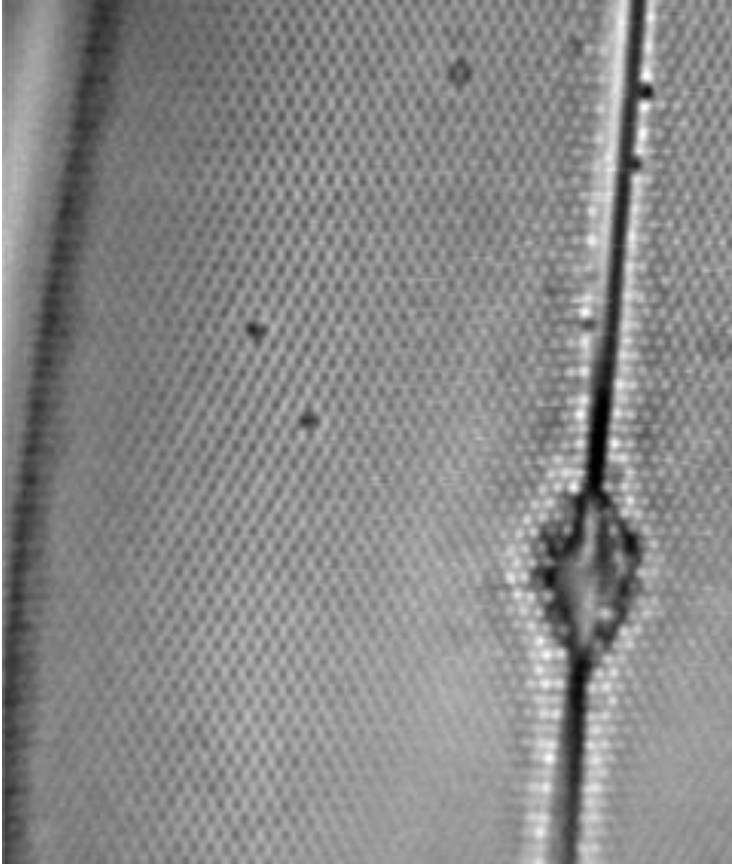


High NA Objective

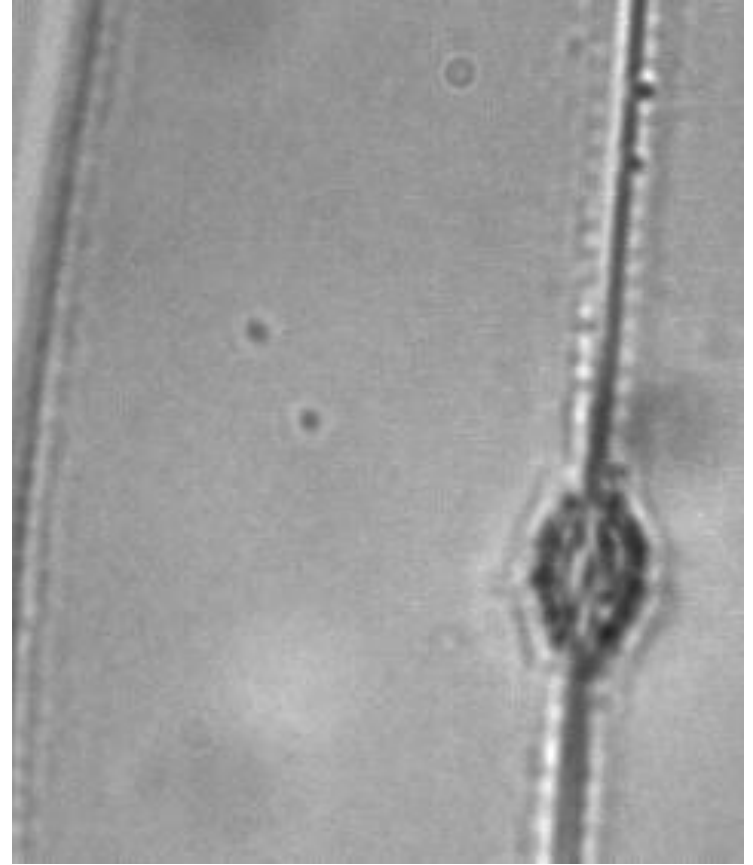

Low NA Objective

Alternate Definitions of Resolution

As the Full Width at Half Max
(FWHM) of the PSF

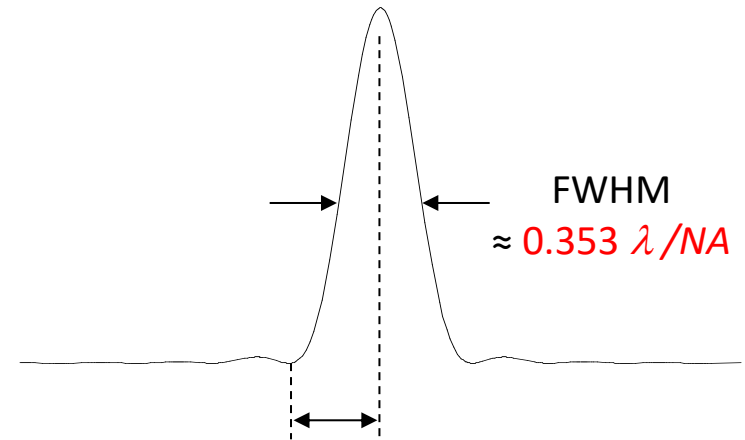

As the diameter of the Airy disk
(first dark ring of the PSF)
= “Rayleigh criterion”

(Probably most common definition)

Airy disk radius
 $\approx 0.61 \lambda / NA$



Objective Types

Field flatness

- Plan or not

Phase rings for phase contrast

- Positive or negative
- Diameter of ring (number)

Special Properties

- Strain free for Polarization or DIC

Features

- Correction collar for spherical aberration
- Iris
- Spring-loaded front end
- Lockable front end

Basic properties

- Magnification
- Numerical Aperture (NA)
- Infinite or finite conjugate
- Cover slip thickness if any
- Immersion fluid if any

Correction class

- Achromat
- Fluor
- Apochromat

Further reading

www.microscopyu.com

micro.magnet.fsu.edu

Douglas B. Murphy “Fundamentals of Light Microscopy and Electronic Imaging”

James Pawley, Ed. “Handbook of Biological Confocal Microscopy, 3rd ed.”

Acknowledgements

Ron Vale / Mats Gustafsson